







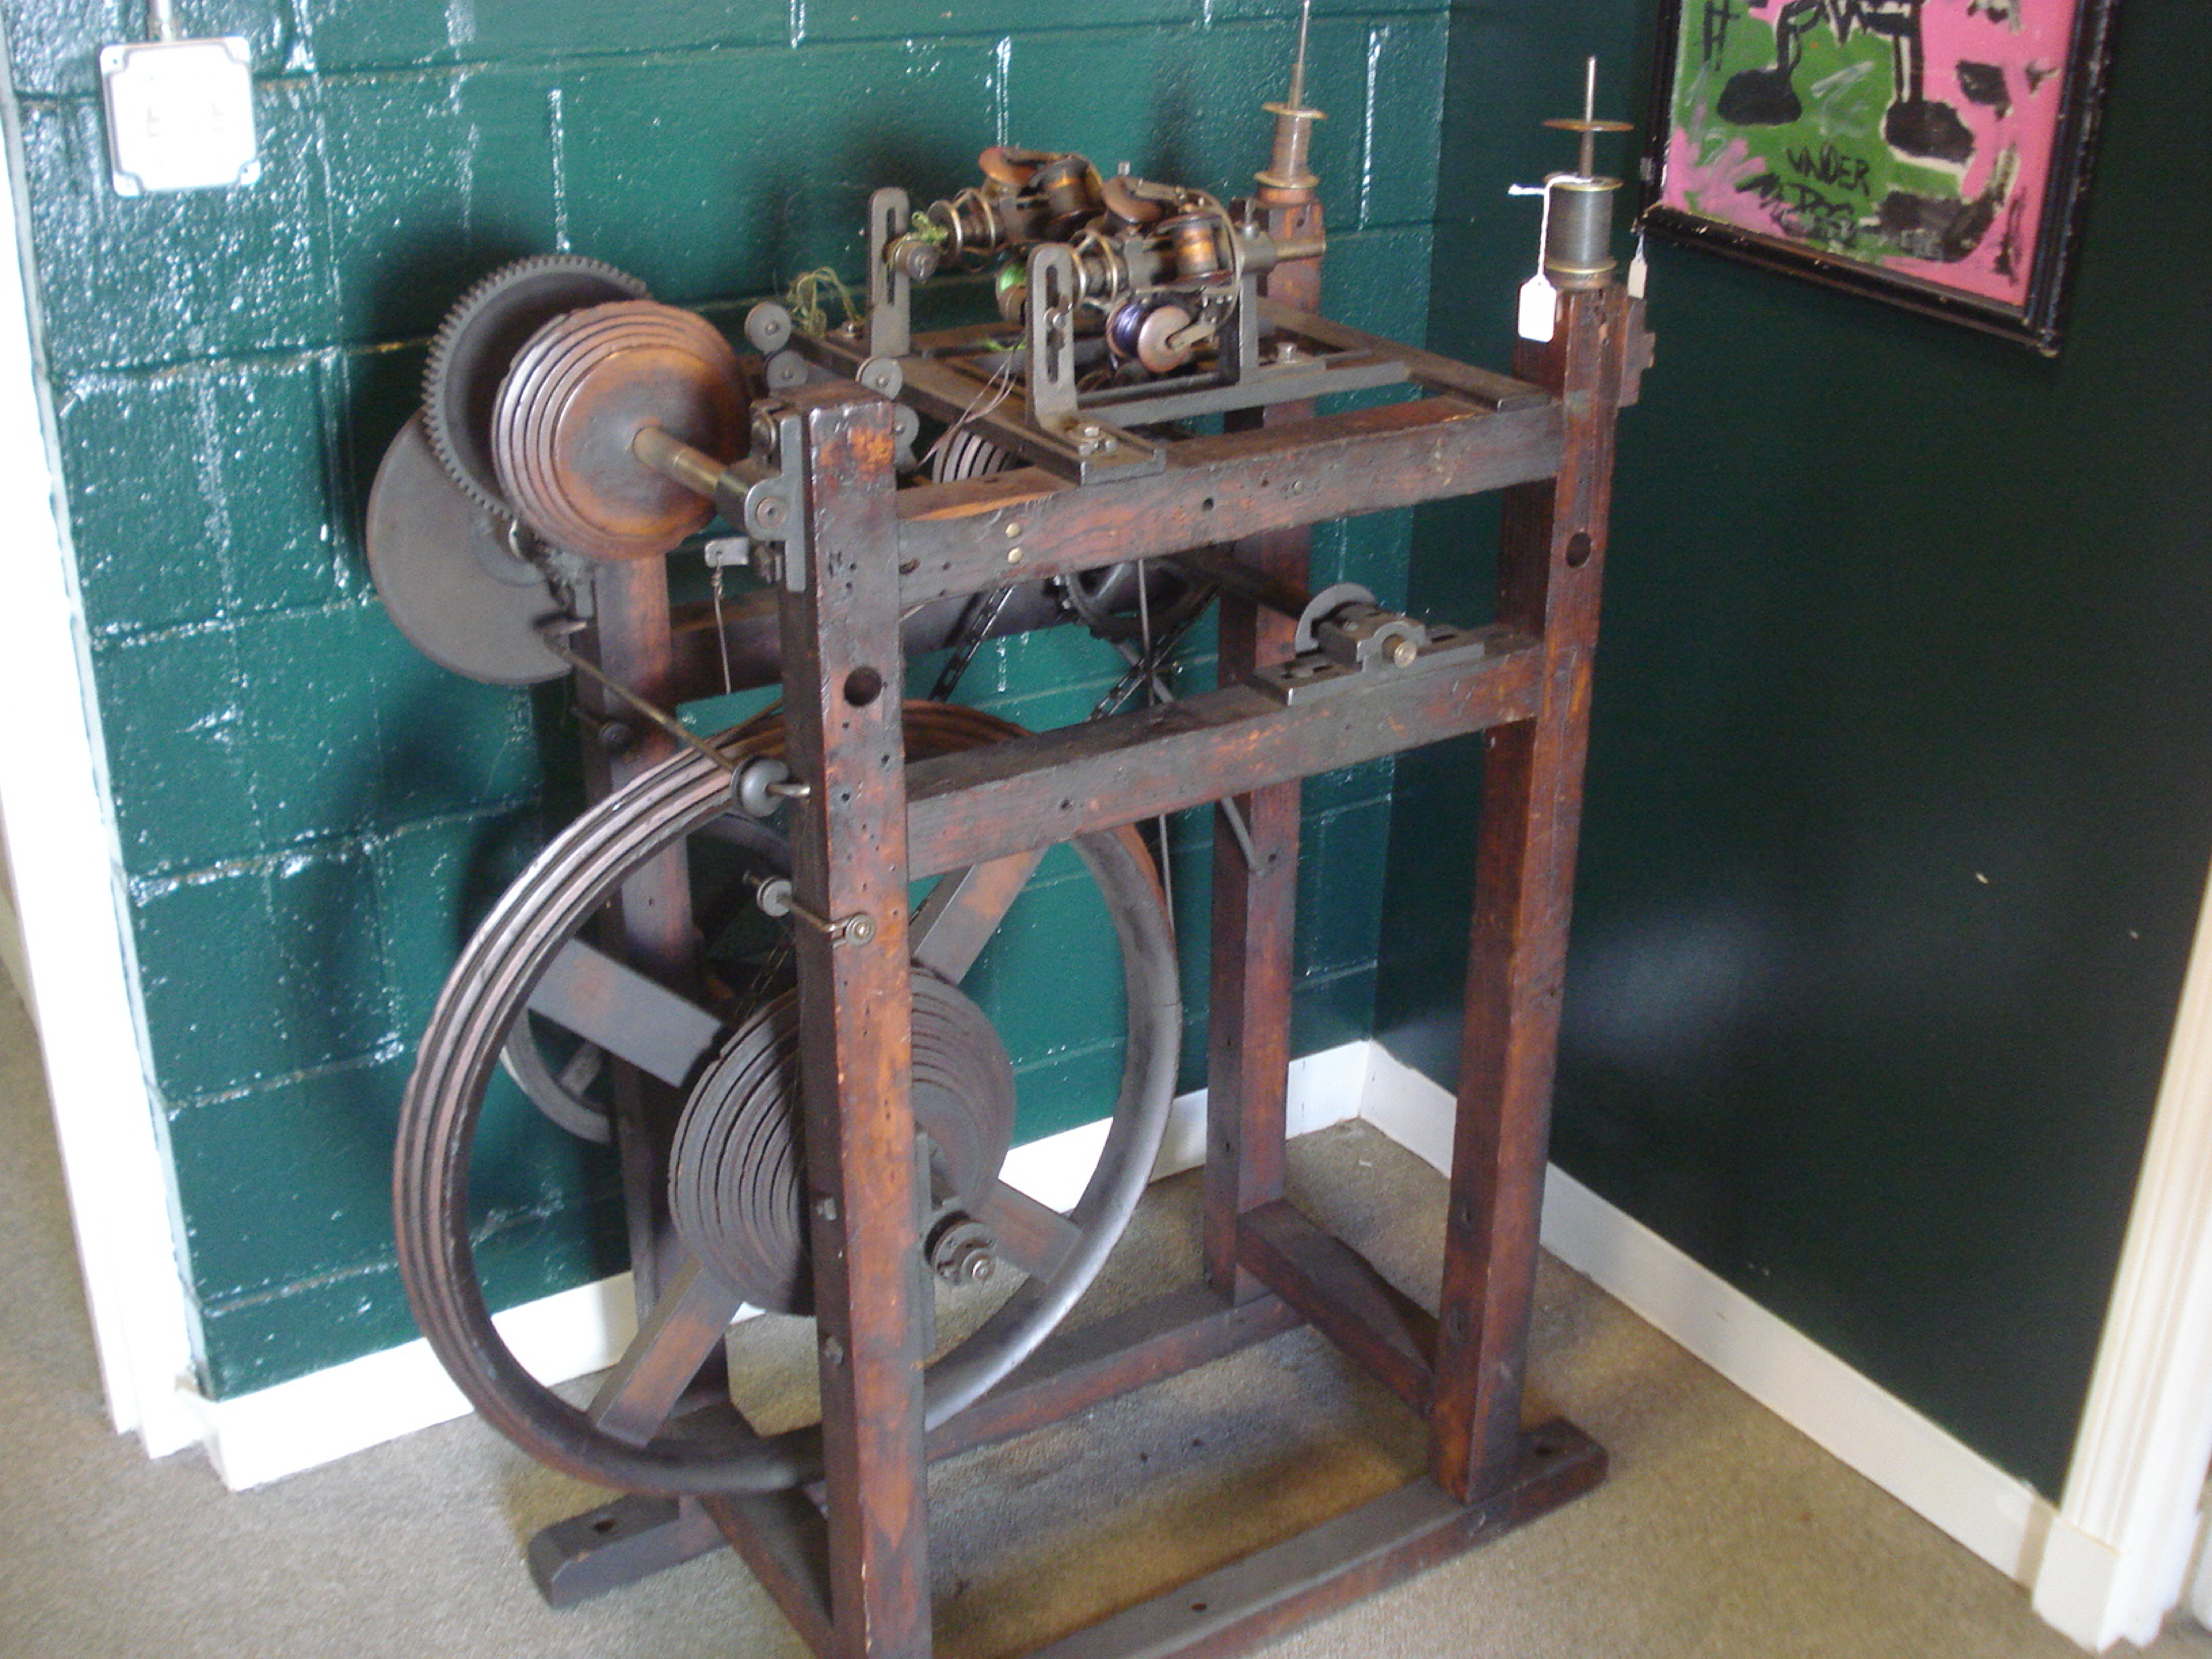

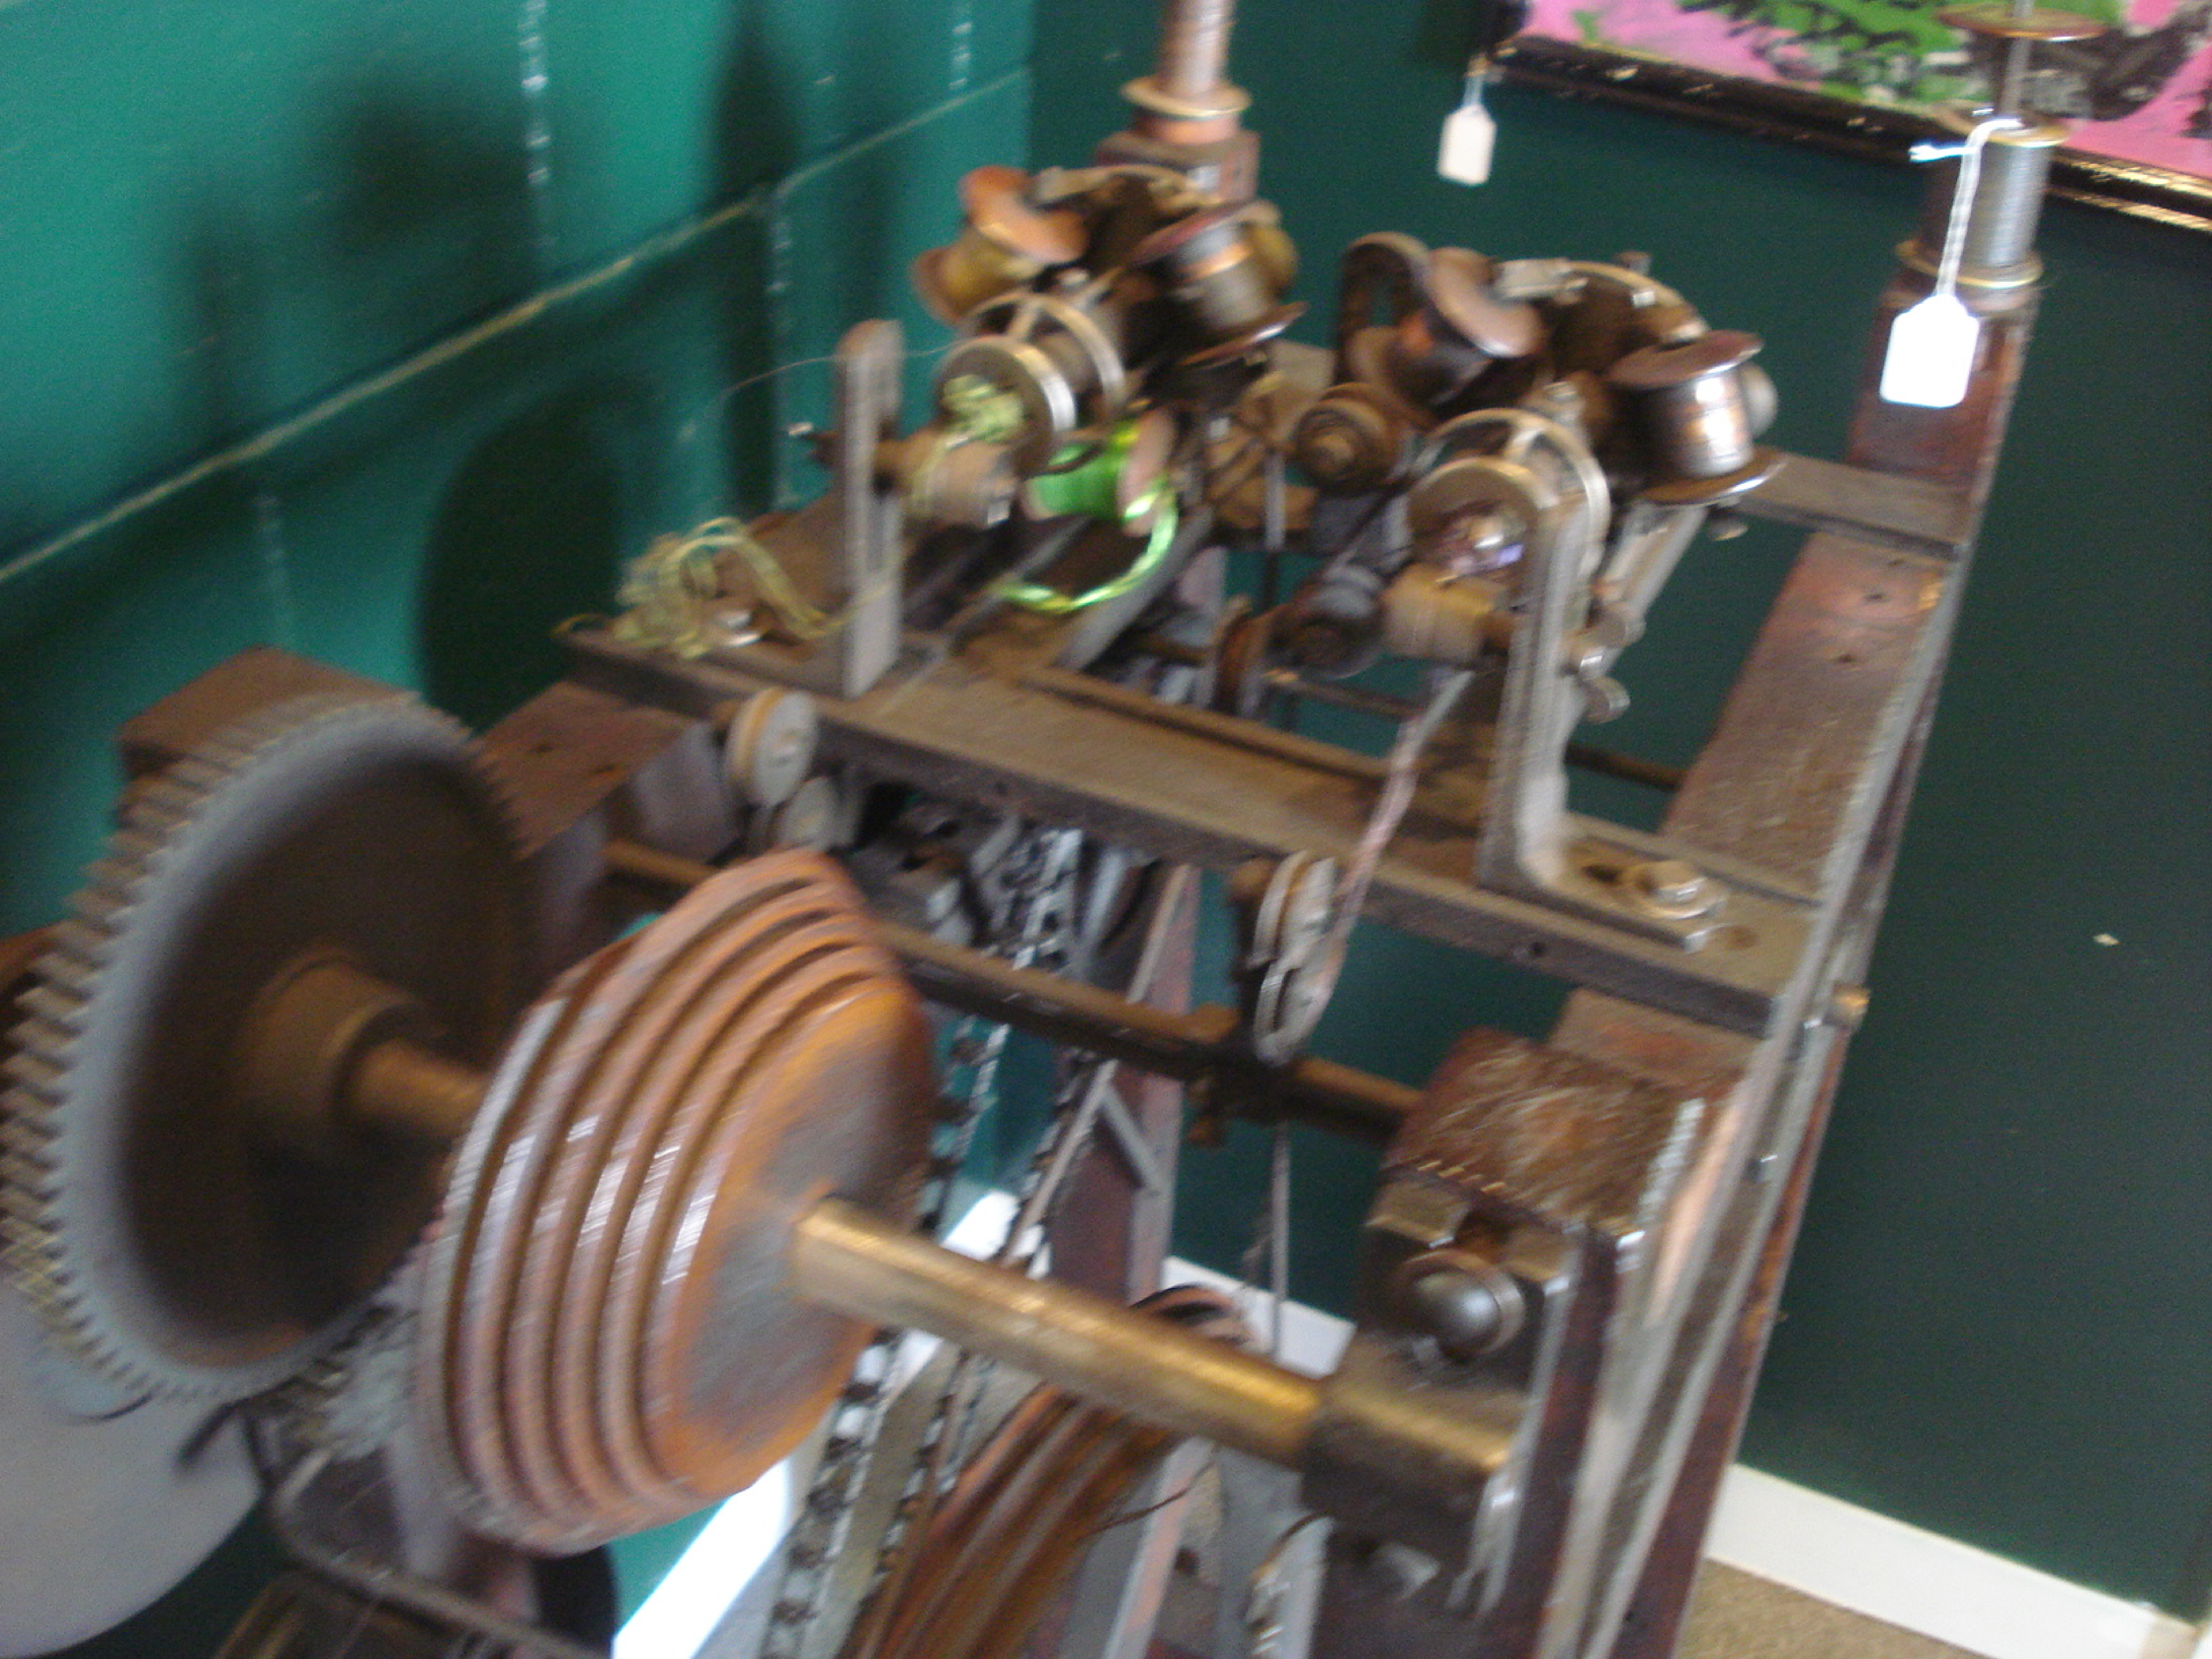


VICTOR
CHICAGO.


ELECTRIC CO. CHICAGO






1052






Do Not


CAUTERY
110 V.
793
4


ELLI BUK MUSEUM COLLECTION
GROGAN & COMPANY
1148
3


ELLI BUK MUSEUM COLLECTION
1148
3
GROGAN & COMPANY


ELLI BUK MUSEUM COLLECTION
1148
3
GROGAN & COMPANY




EXIT





HELIOTONE
TRADE MARK REG. U. S. PAT. OFF.
THERAPEUTIC LAMP
FRANK S. BETZ CO.
HAMMOND, IND.
V. 110 CY. AMP. 10 TYPE NO. 56576






HALLIWELL-SHELTON
GIANT SPECIAL
TYPE 100
MODEL 28270
VOLTS 110 V AC & DC
AMPS 1.25
SER. 1732
HALLIWELL-SHELTON ELEC. CORP.
NEW YORK
CHICAGO



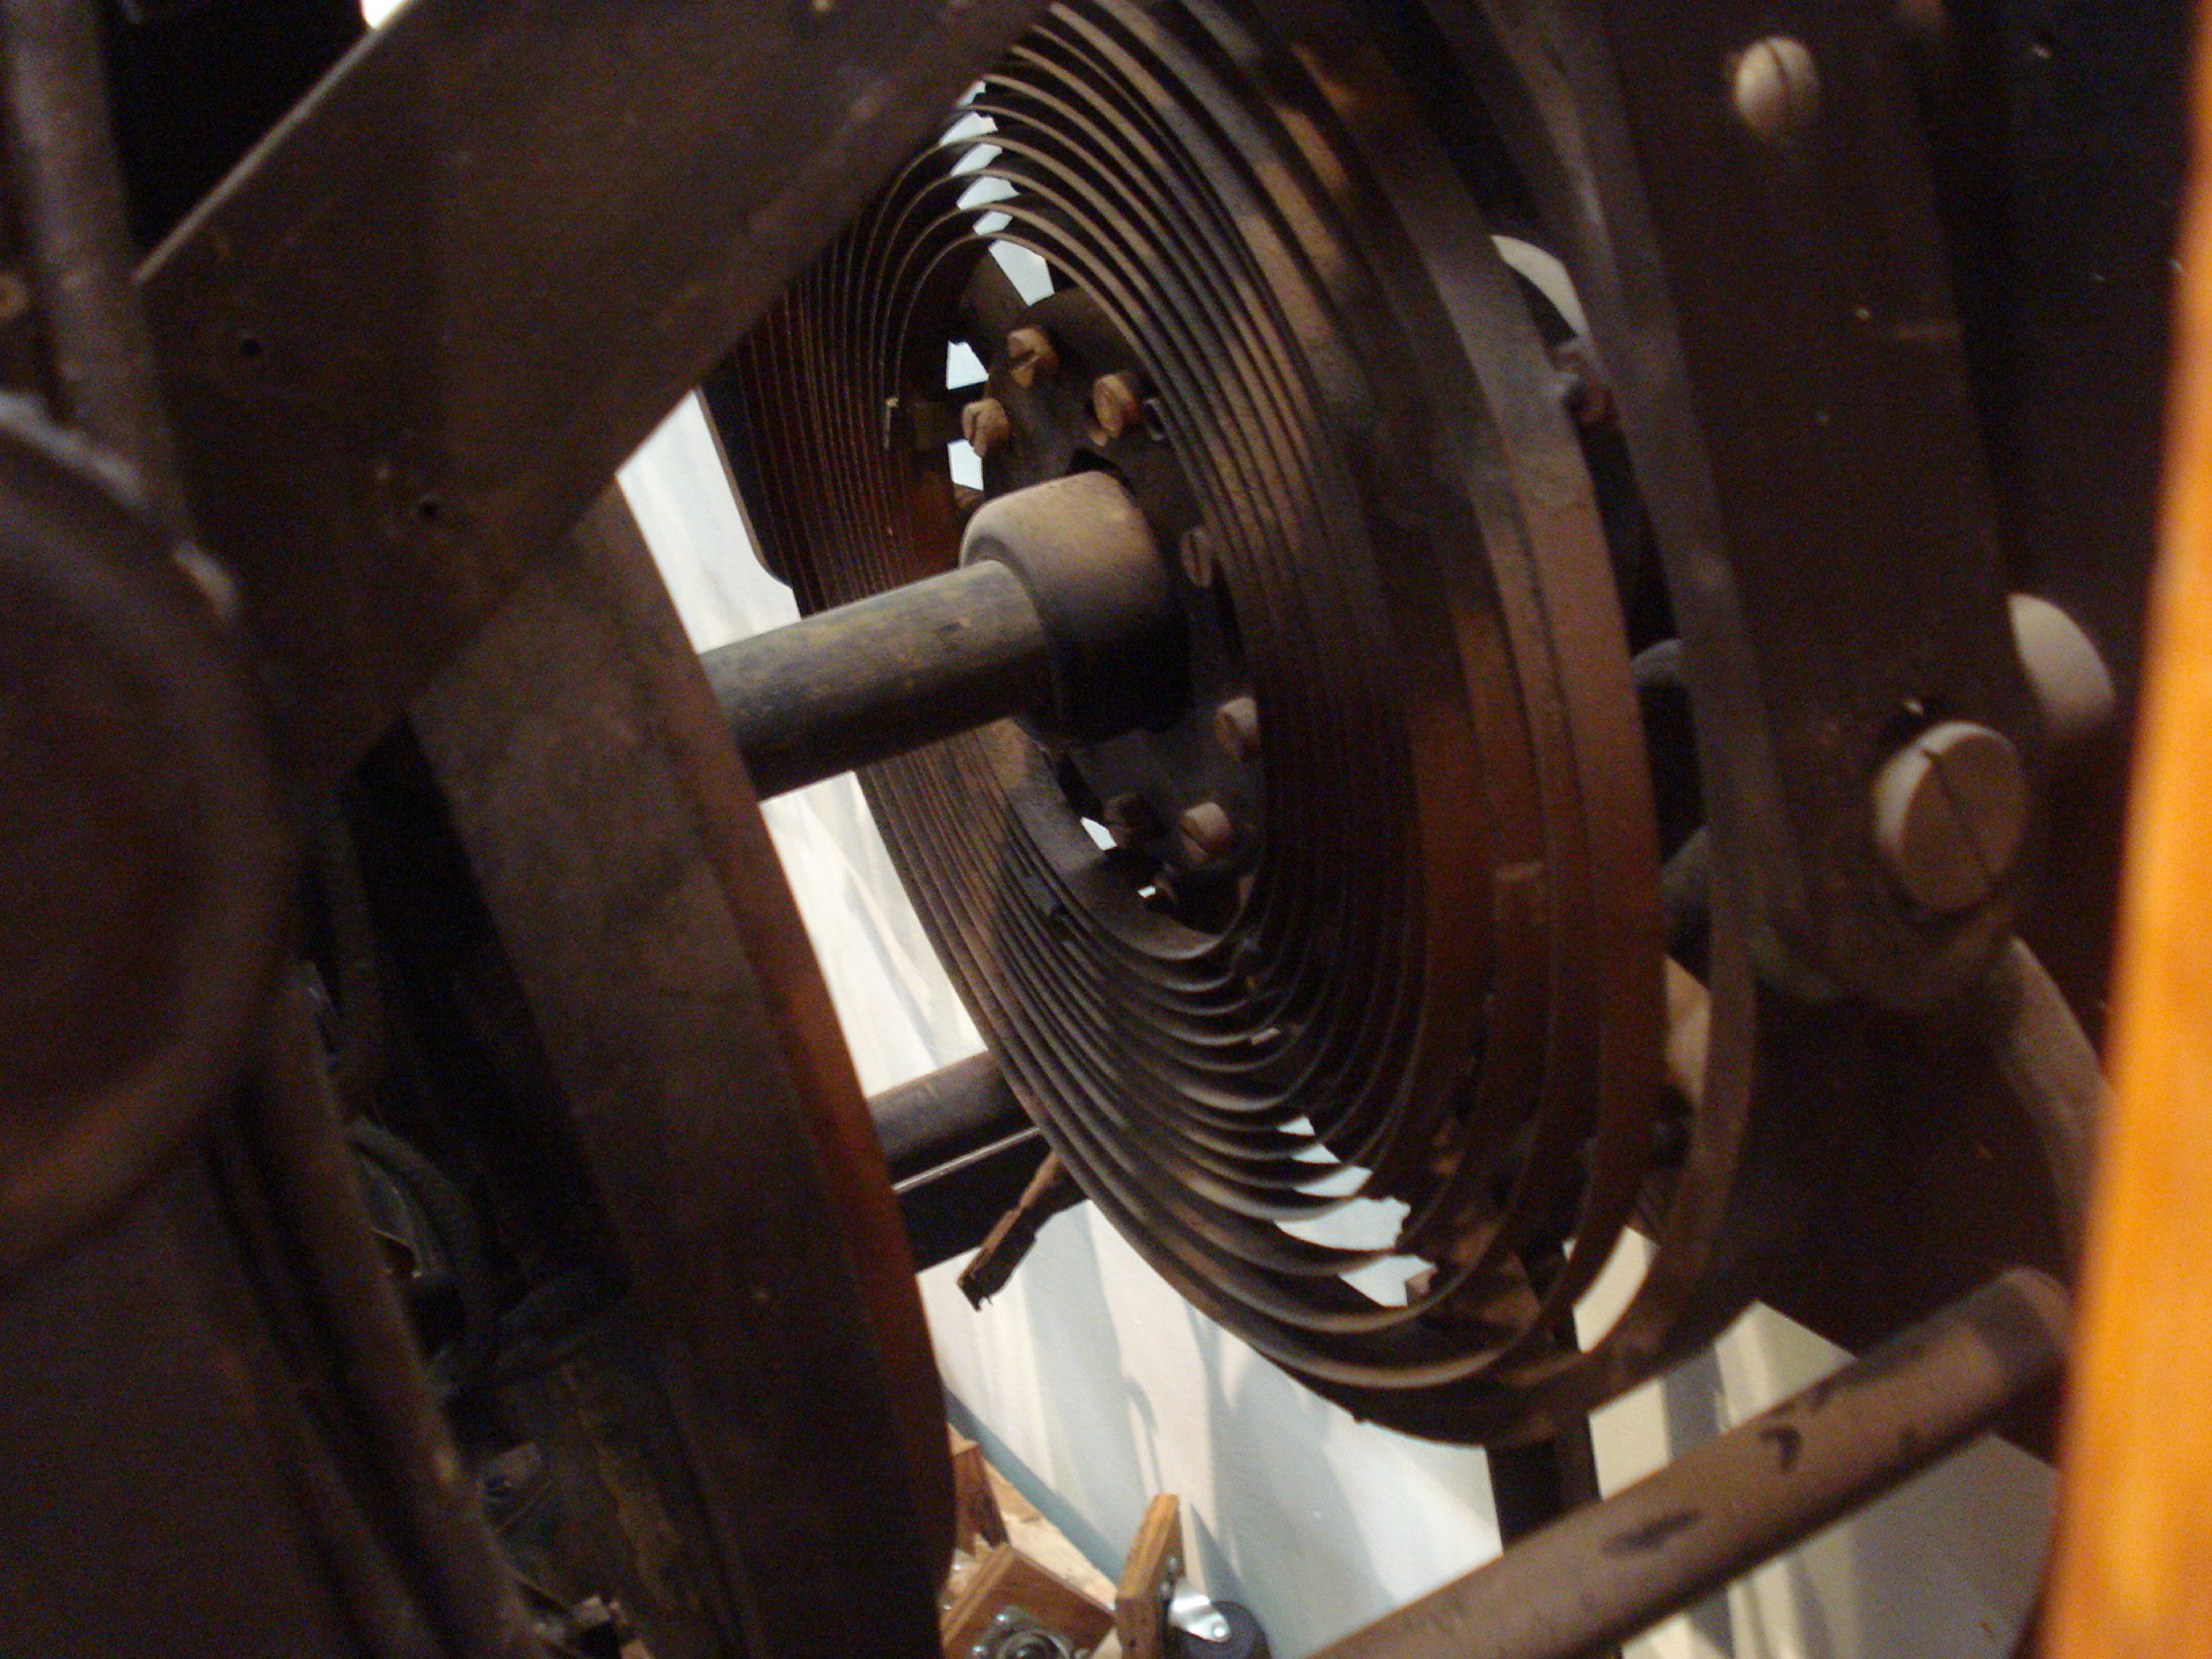


WESTON
VOLTS
WESTON ELECTRICAL INSTRUMENT CO.
NEWARK N.J. U.S.A.
VOLTMETER
A.C.
WESTON
WATTS
CV 520
WESTON ELECTRICAL INSTRUMENT CO.
NEWARK N.J. U.S.A.
375 K.C.
545 K.C.


SE 1001
SE 1001
SE 1001
SE 1001





S.E. 1001



SPECTRO-CHROME INSTITUTE
DINSHAH-ATTUNED COLOR WAVES



SPECTRO-CHROME METRY
MEASUREMENT AND RESTORATION OF THE HUMAN
RADIO-ACTIVE AND RADIO-EMANATIVE EQUILIBRIUM
(NORMALATION OF IMBALANCE)
BY
ATTUNED COLOR WAVES
THE SCIENCE OF AUTOMATIC PRECISION
NO DIAGNOSIS – NO DRUGS – NO MANIPULATION – NO SURGERY
CONCEIVED, ORIGINATED, DEVELOPED, APPLIED & COPYRIGHTED 1920 BY
COLONEL DINSHAH P. GHADIALI, M.D., M.E., D.C., PH.D., LL.D.
METAPHYSICIAN AND PSYCHOLOGIST
YELLOW
ORANGE
BLUE
INDIGO
VIOLET
MAGENTA
SPECTRO-CHROME
TRADE MARKS
Dinshah
REG. U.S. PAT. OFF
UA-4627
U.S. PATENT NUMBER
MANUFACTURED IN U.S. AMERICA BY
SPECTRO-CHROME INSTITUTE
(INCORPORATED)
CENTRAL OFFICE
MALAGA, NEW JERSEY
RESEARCH LABORATORY
UNDERSTANDING
AS THE PROPER USE OF THIS SPECTRO-CHROME REQUIRES SPECIAL TRAINING AND TECHNICAL KNOWLEDGE IN THE USER AND ALSO NECESSITATES THE PRODUCTION OF THE ATTUNED COLOR WAVES BY MEANS OF THE GENUINE DINSHAH ATTUNED COLOR WAVE SLIDES, THIS APPARATUS IS SOLD WITHOUT ANY LIABILITY, GUARANTEE OR WARRANTY, EXPRESSED OR IMPLIED, REGARDING THE RESULTS ATTAINABLE AND ITS PURCHASE OR POSSESSION DOES NOT CONFER ON THE PURCHASER OR POSSESSOR ANY TITLE, DESIGNATION OR DEGREE PERTAINING TO THE PRACTICE OF SPECTRO-CHROME METRY OR OBLIGATE THE SPECTRO-CHROME INSTITUTE IN ANY MANNER.

SPECTRO-CHROME METRY
MEASUREMENT AND RESTORATION OF THE HUMAN
RADIO-ACTIVE AND RADIO-EMANATIVE EQUILIBRIUM
(NORMALATION OF IMBALANCE)
BY
ATTUNED COLOR WAVES
THE SCIENCE OF AUTOMATIC PRECISION
NO DIAGNOSIS – NO DRUGS – NO MANIPULATION – NO SURGERY
CONCEIVED, ORIGINATED, DEVELOPED, APPLIED & COPYRIGHTED 1920 BY
COLONEL DINSHAH P. GHADIALI, M.D., M.E., D.C., PH.D., LL.D.
METAPHYSICIAN AND PSYCHOLOGIST
SPECTRO-CHROME
TRADE MARKS
REG. U.S. PAT. OFF.
Dinshah
EQUIPMENT NUMBER
UA-4627
U.S. PATENT NUMBER
1544973 - JULY 7, 1925
MANUFACTURED IN U.S. AMERICA BY
SPECTRO-CHROME INSTITUTE
(INCORPORATED)
MALAGA, NEW JERSEY
CENTRAL OFFICE
RESEARCH LABORATORY
UNDERSTANDING
AS THE PROPER USE OF THIS SPECTRO-CHROME REQUIRES SPECIAL TRAINING AND TECHNICAL KNOWLEDGE IN THE USER AND ALSO NECESSITATES THE PRODUCTION OF THE ATTUNED COLOR WAVES BY MEANS OF THE GENUINE DINSHAH ATTUNED COLOR WAVE SLIDES, THIS APPARATUS IS SOLD WITHOUT ANY LIABILITY, GUARANTEE OR WARRANTY, EXPRESSED OR IMPLIED, REGARDING THE RESULTS ATTAINABLE AND ITS PURCHASE OR POSSESSION DOES NOT CONFER ON THE PURCHASER OR POSSESSOR ANY TITLE, DESIGNATION OR DEGREE PERTAINING TO THE PRACTICE OF SPECTRO-CHROME METRY OR OBLIGATE THE SPECTRO-CHROME INSTITUTE IN ANY MANNER.



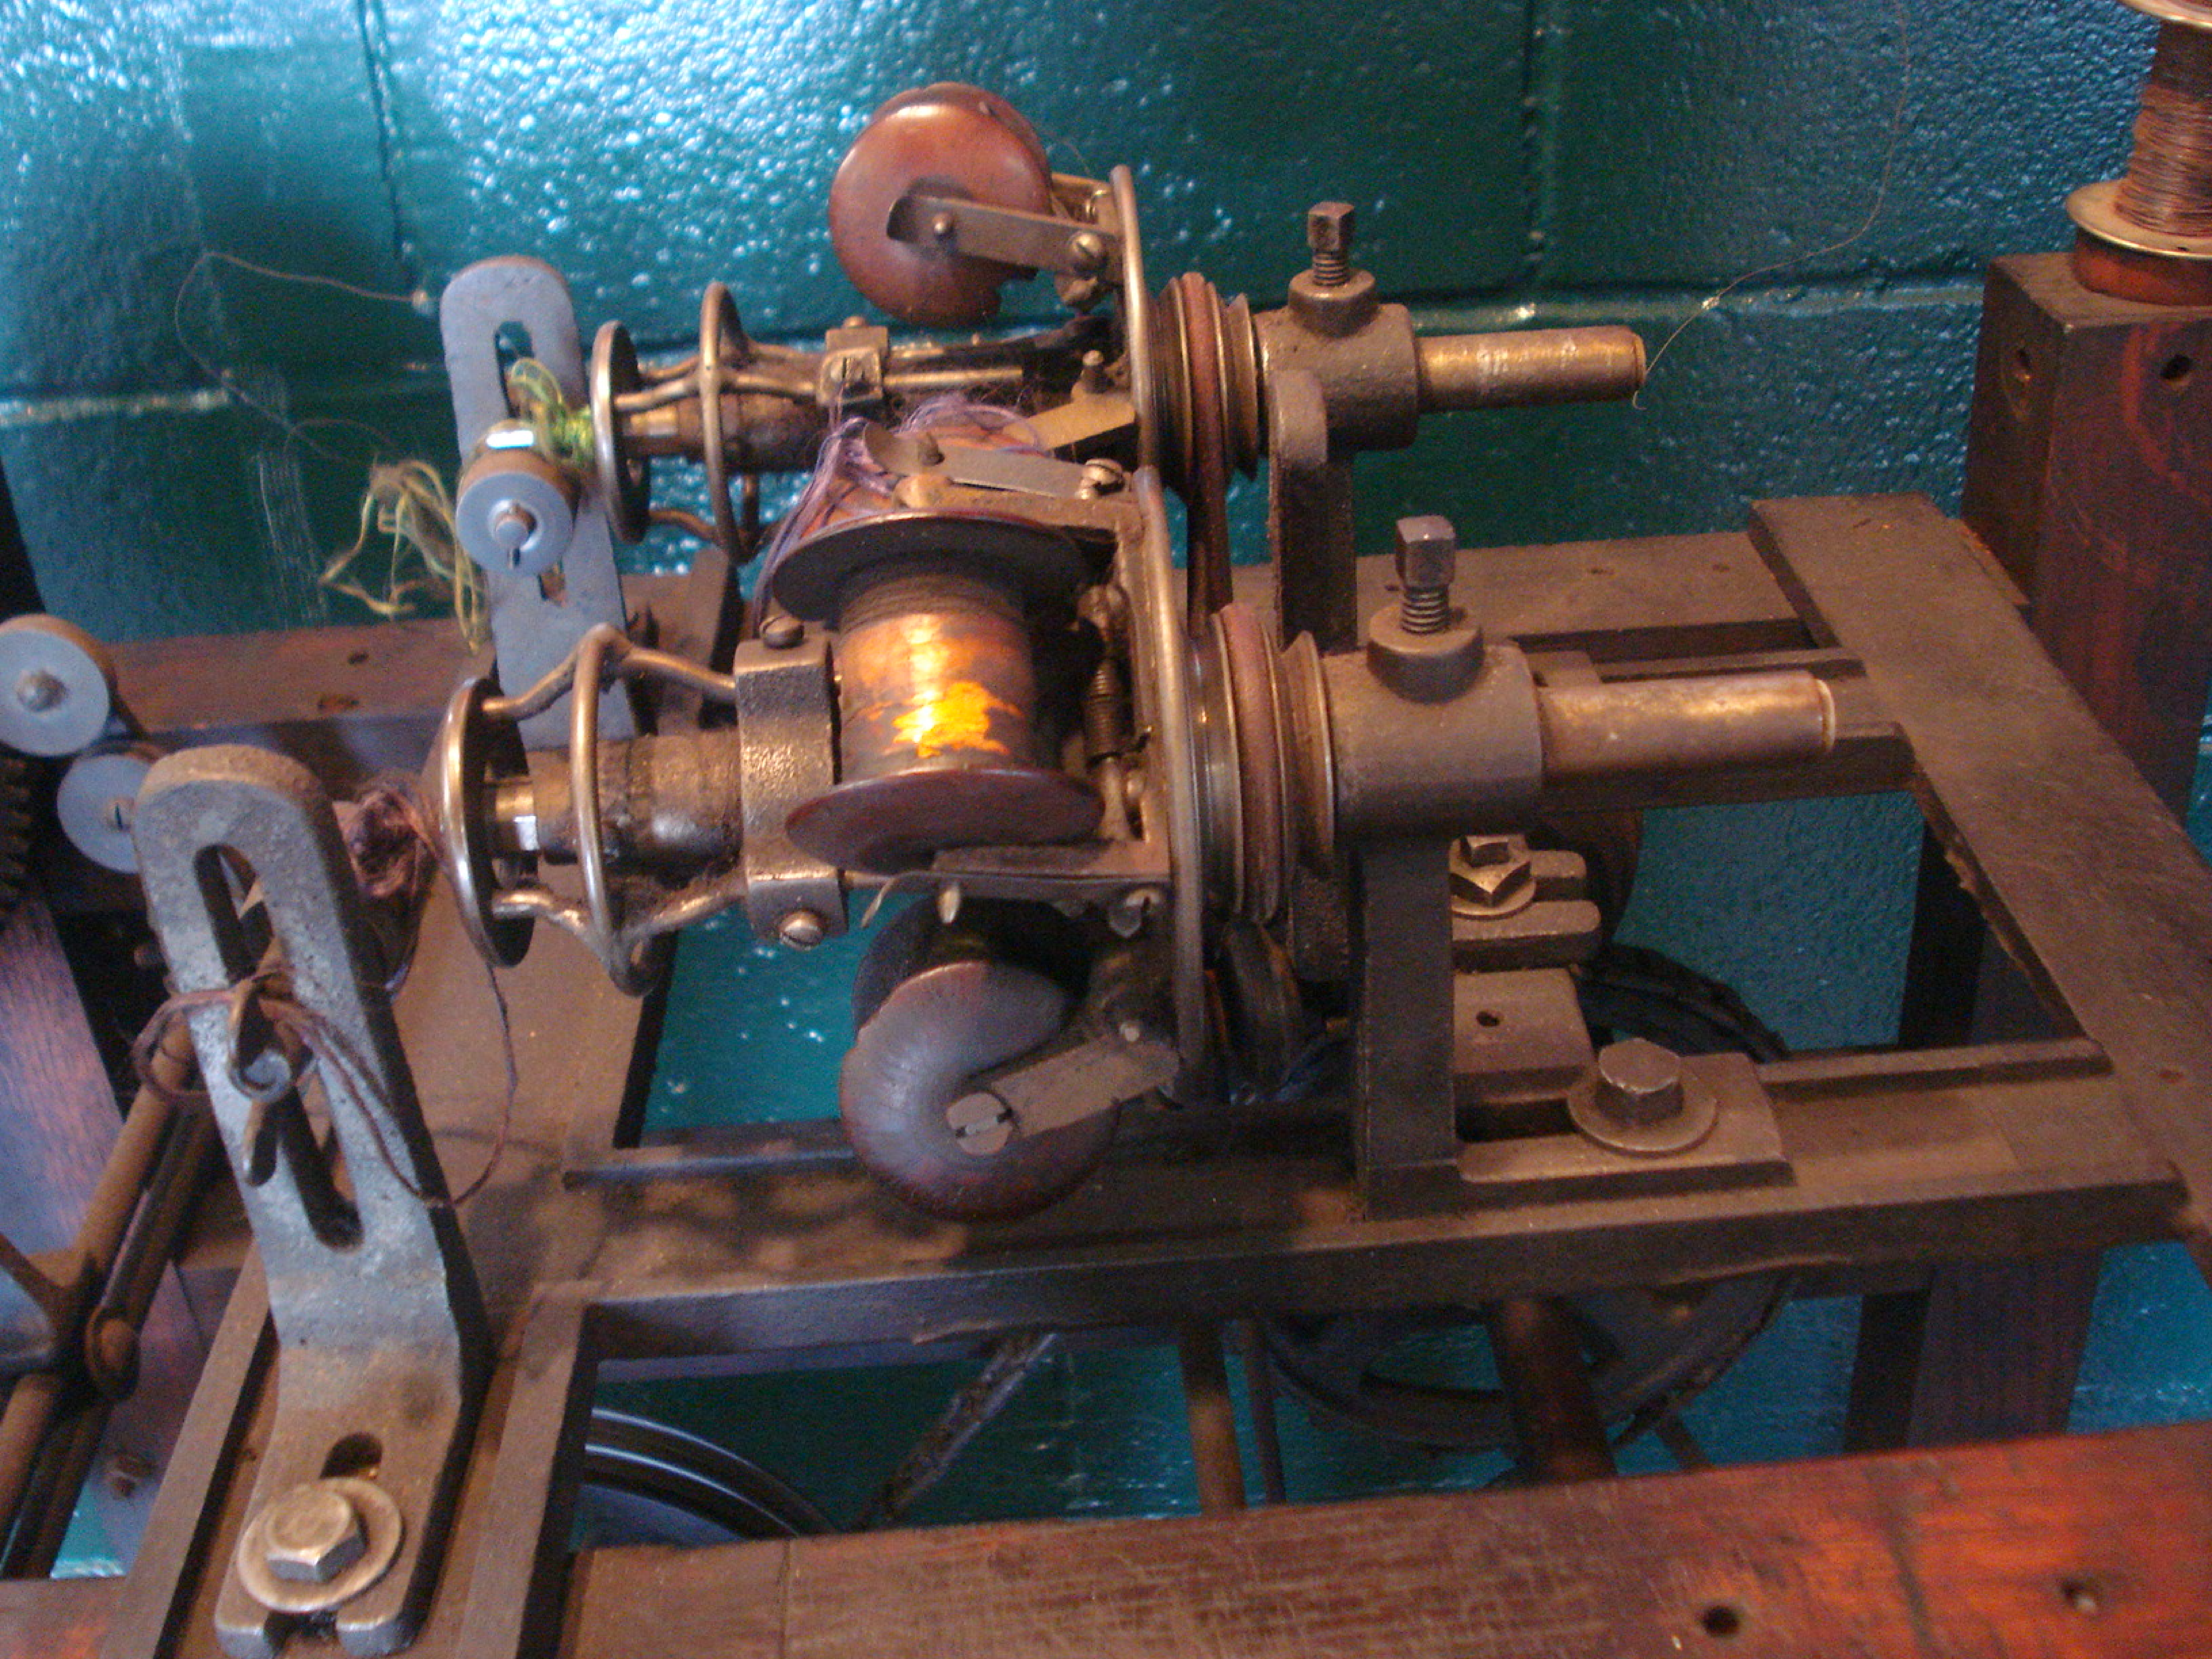


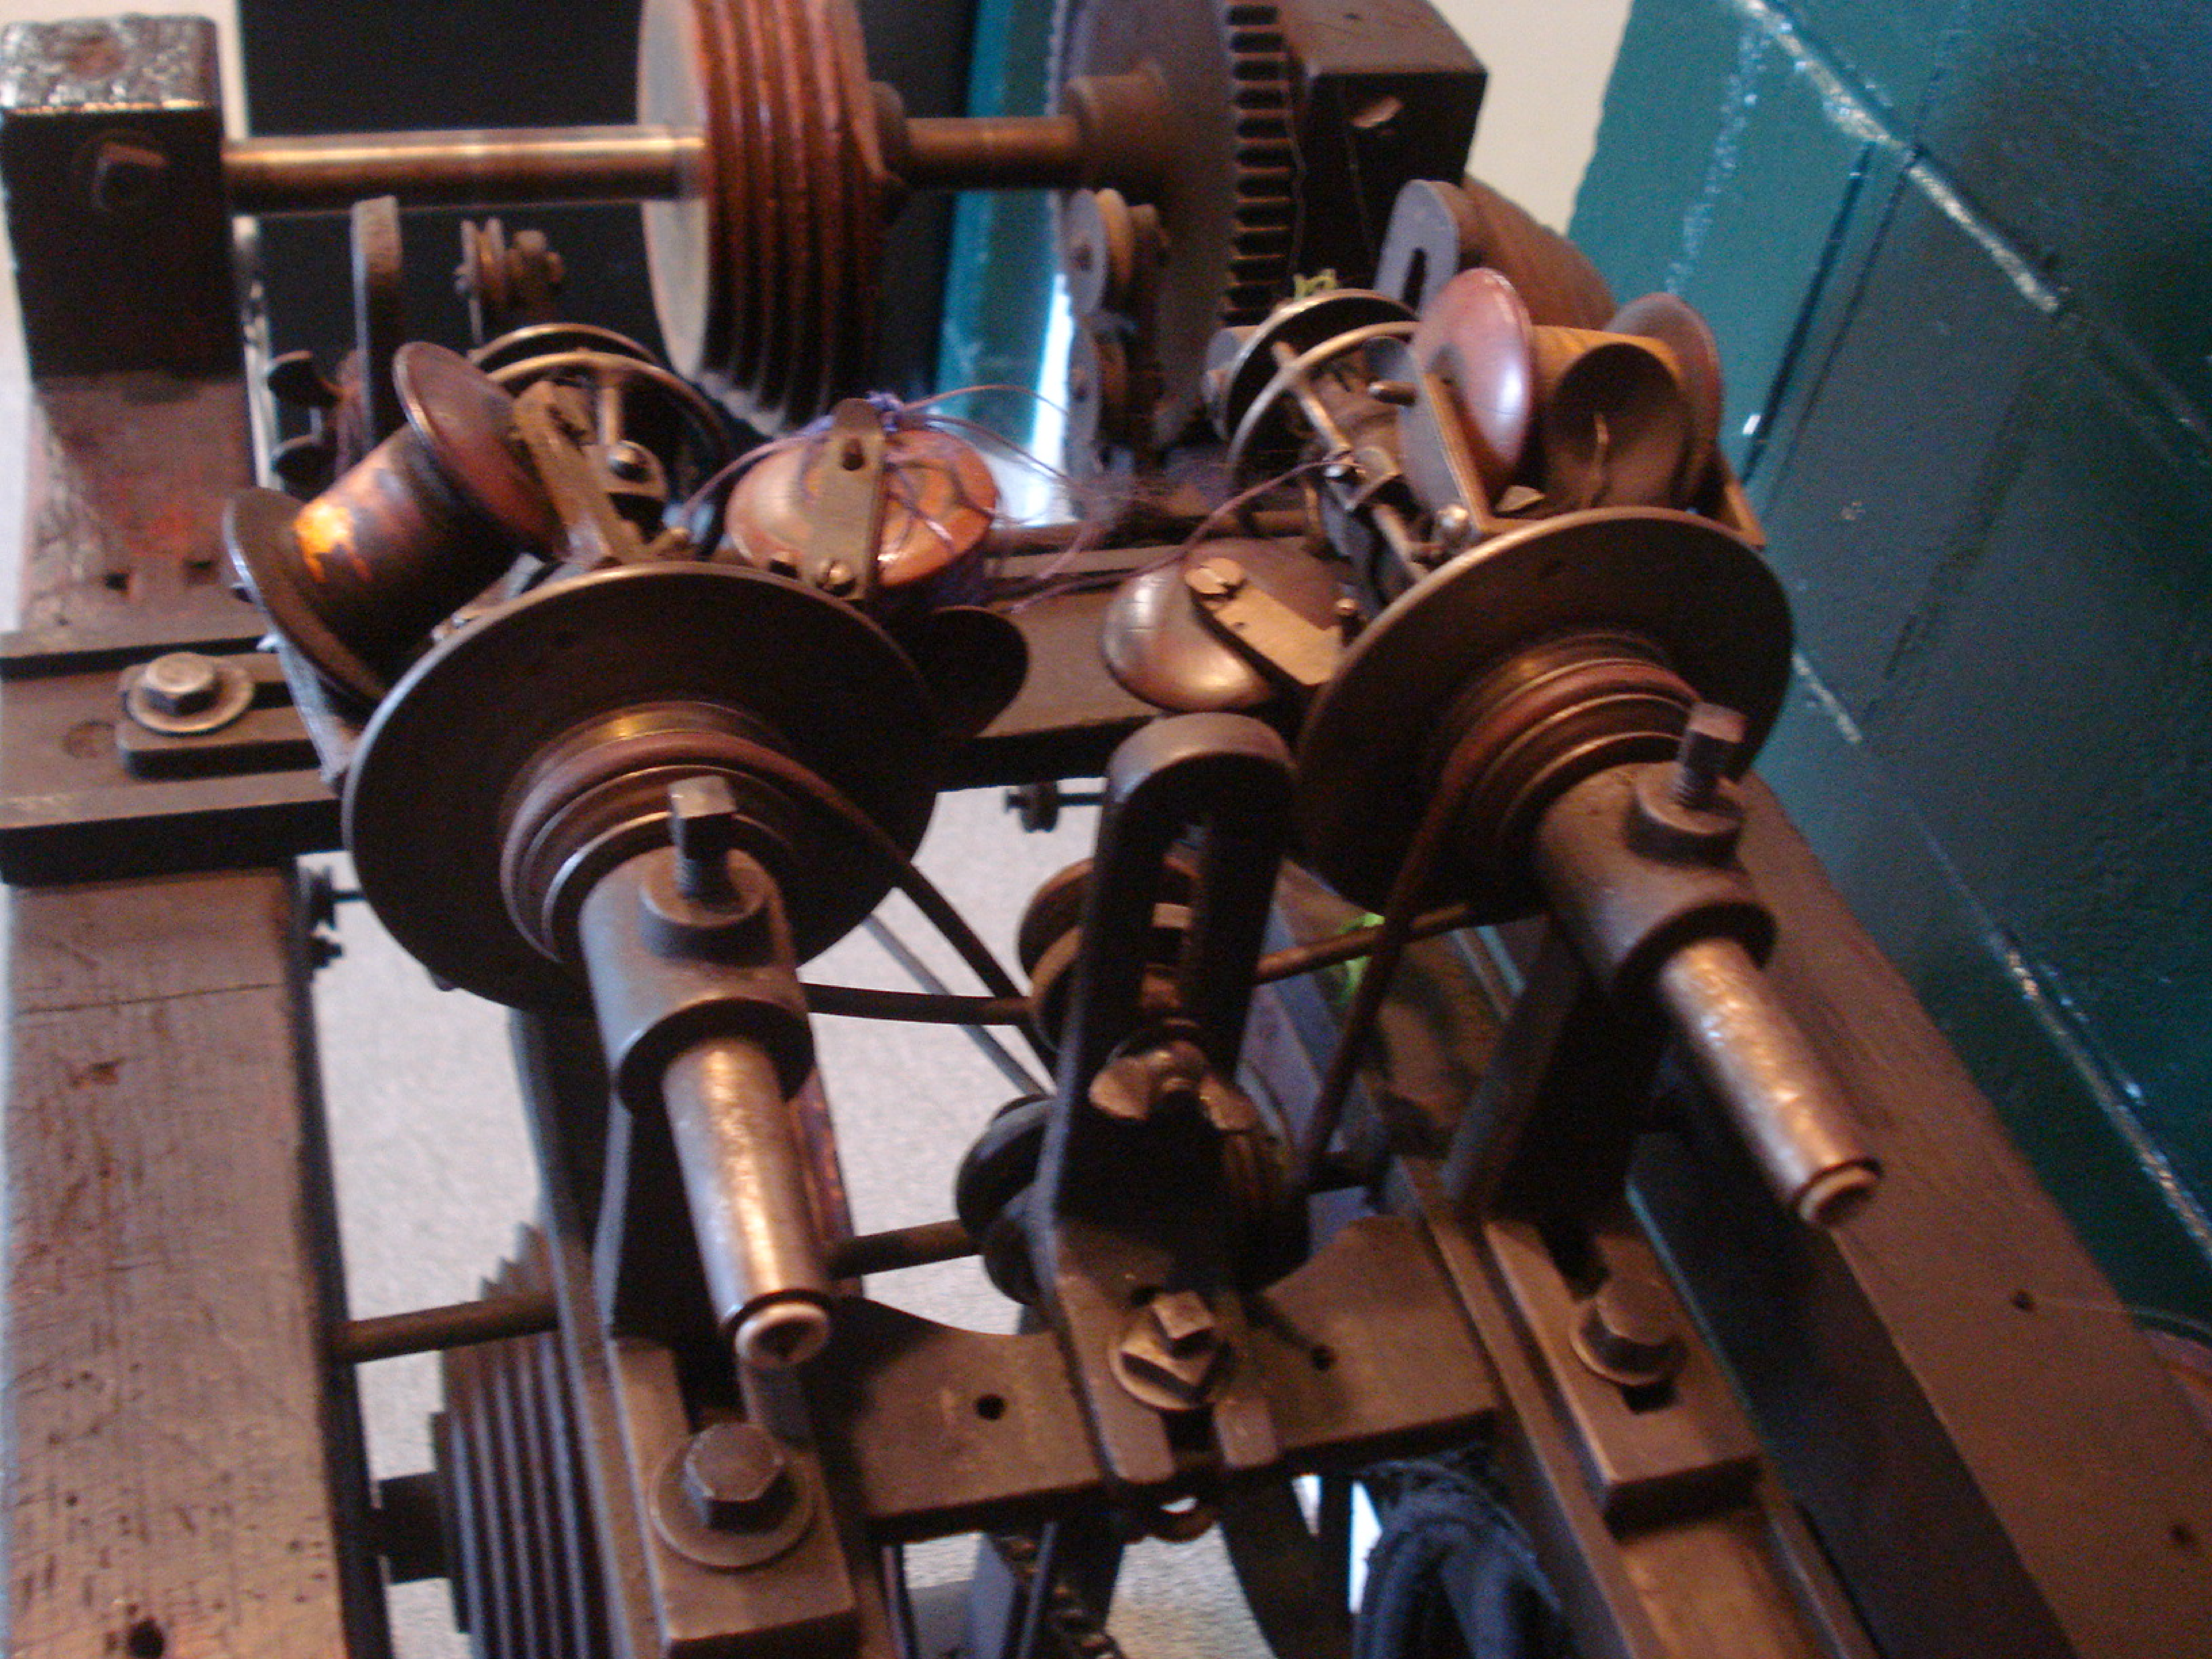

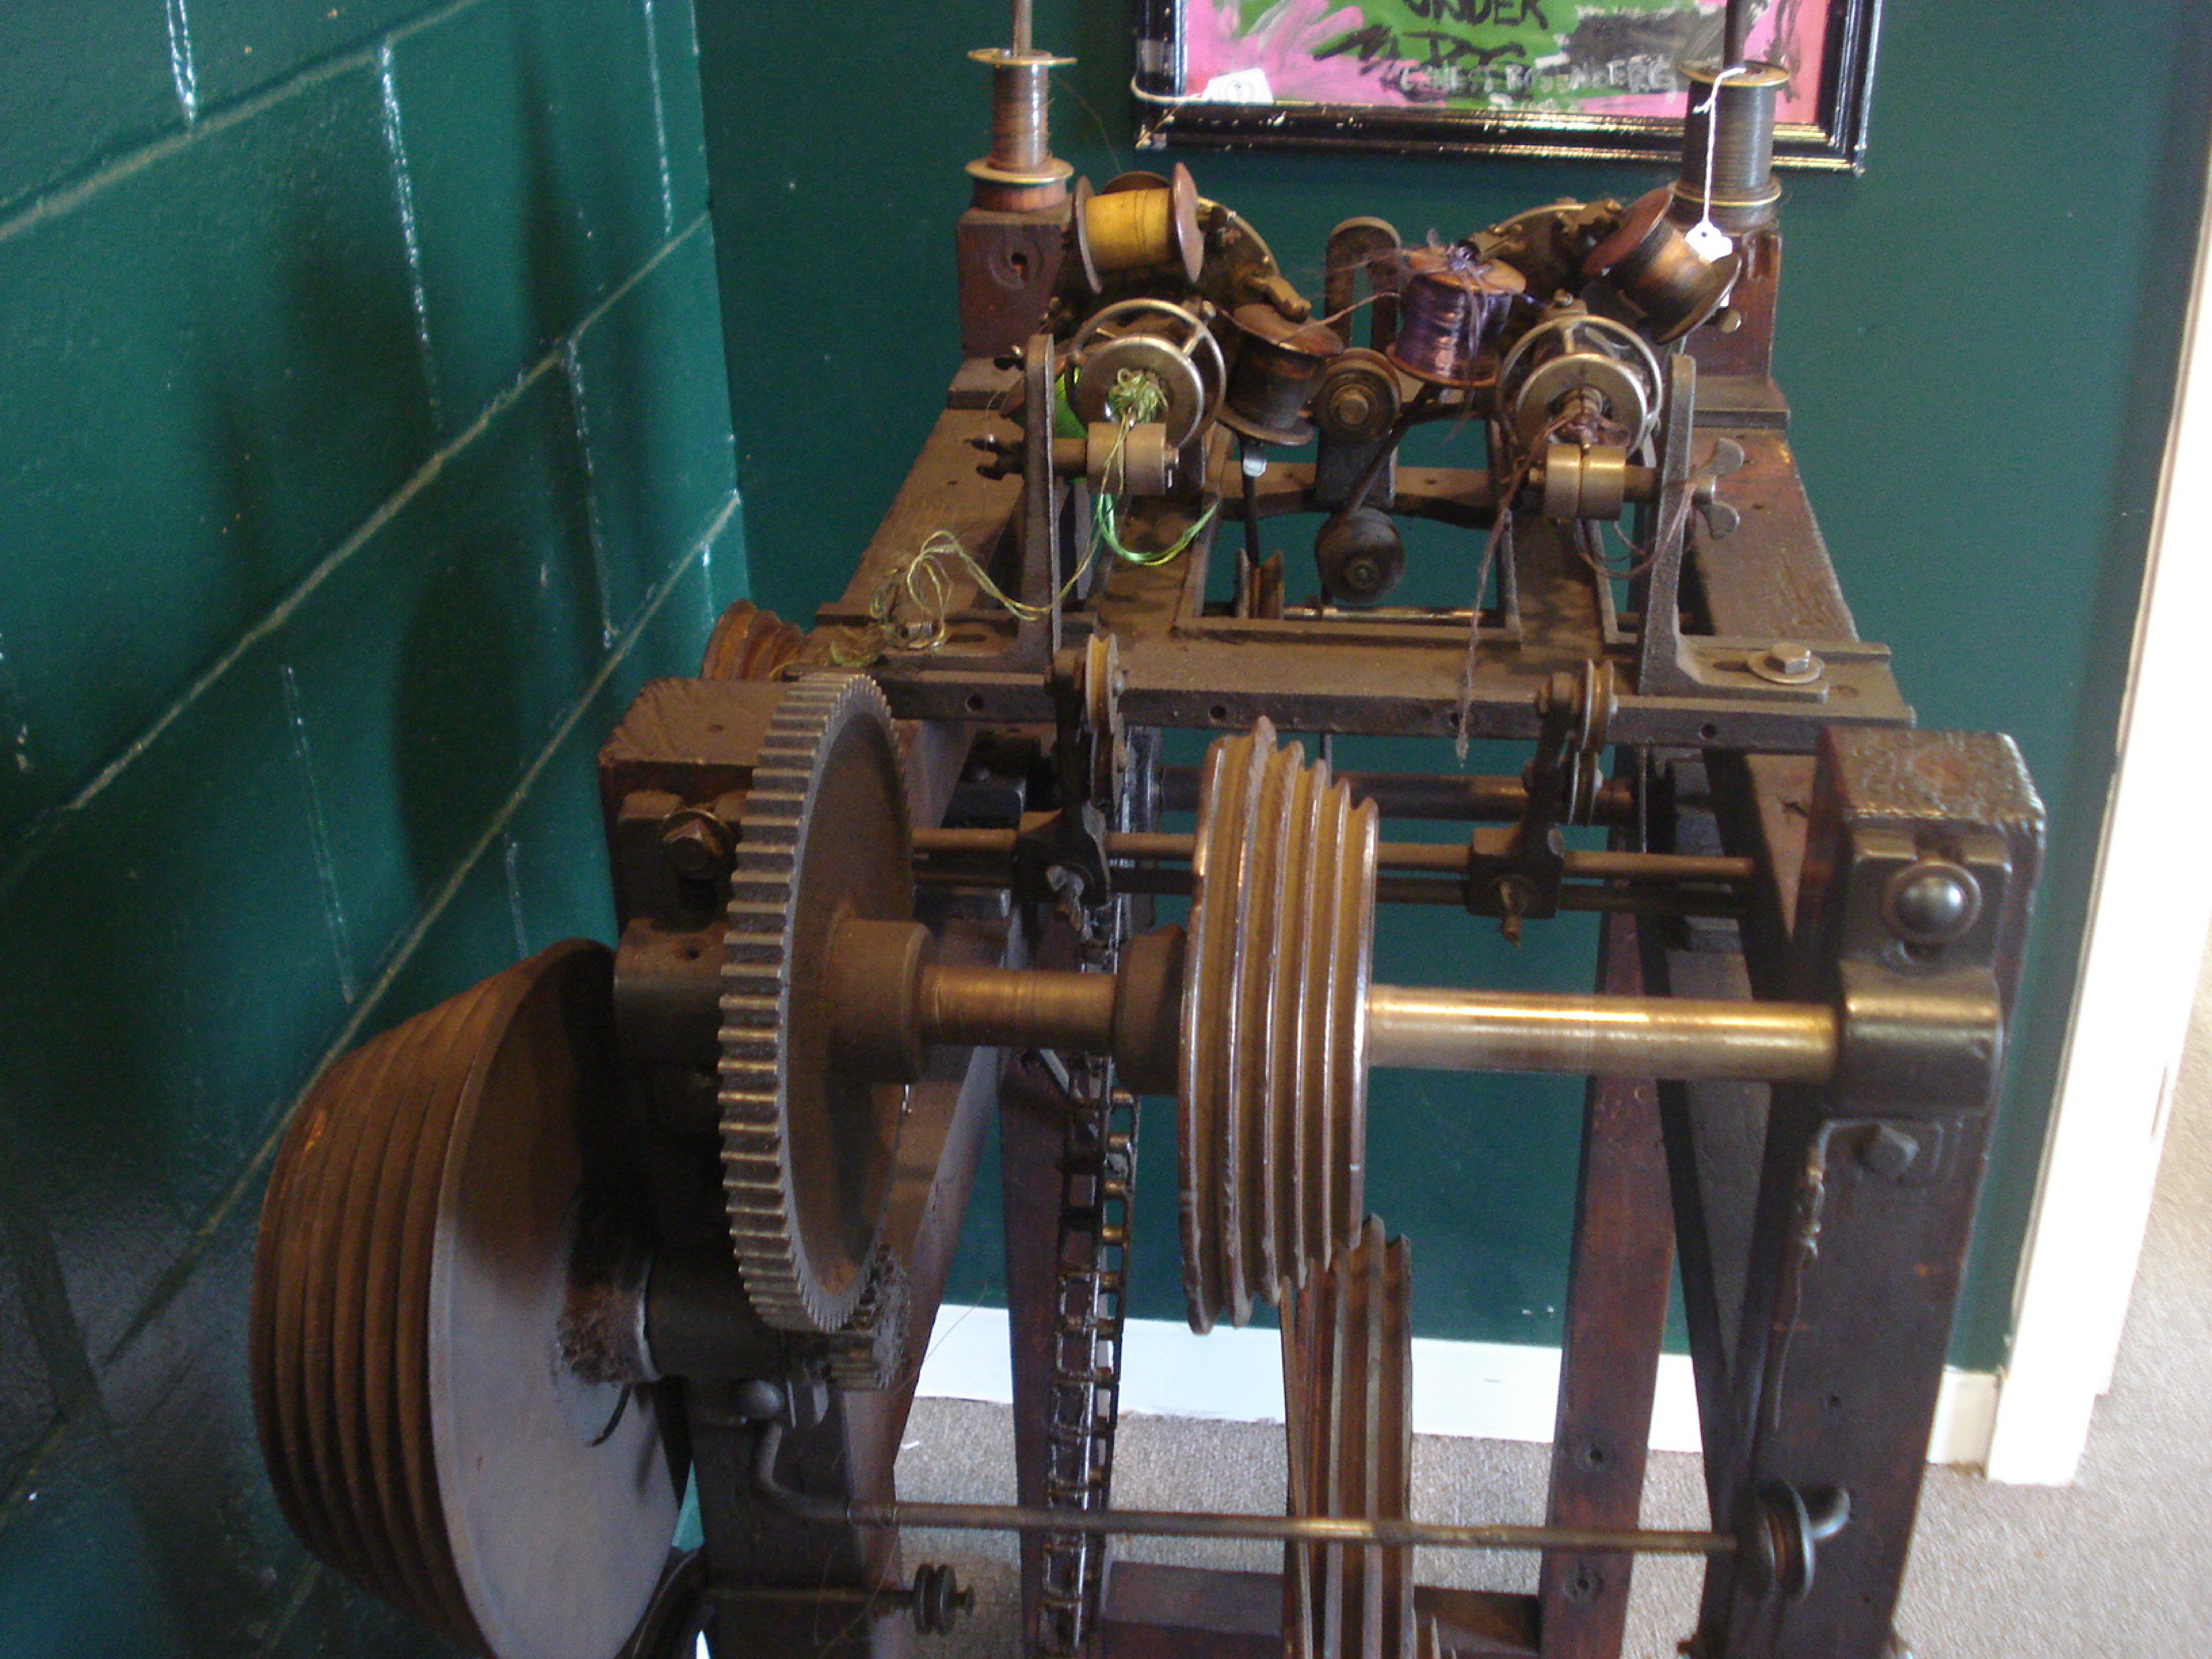




"SUPER DIATHERM"
PHYSIO-THERAPY APPARATUS
A. S. ALOE CO., ST. LOUIS, MO.
SERIAL No. 779 ALTERNATING CURRENT
AMPS 5.5 VOLTS 110 CYCLES 60
MILLIAMPERES
LINE
FOOT SWITCH

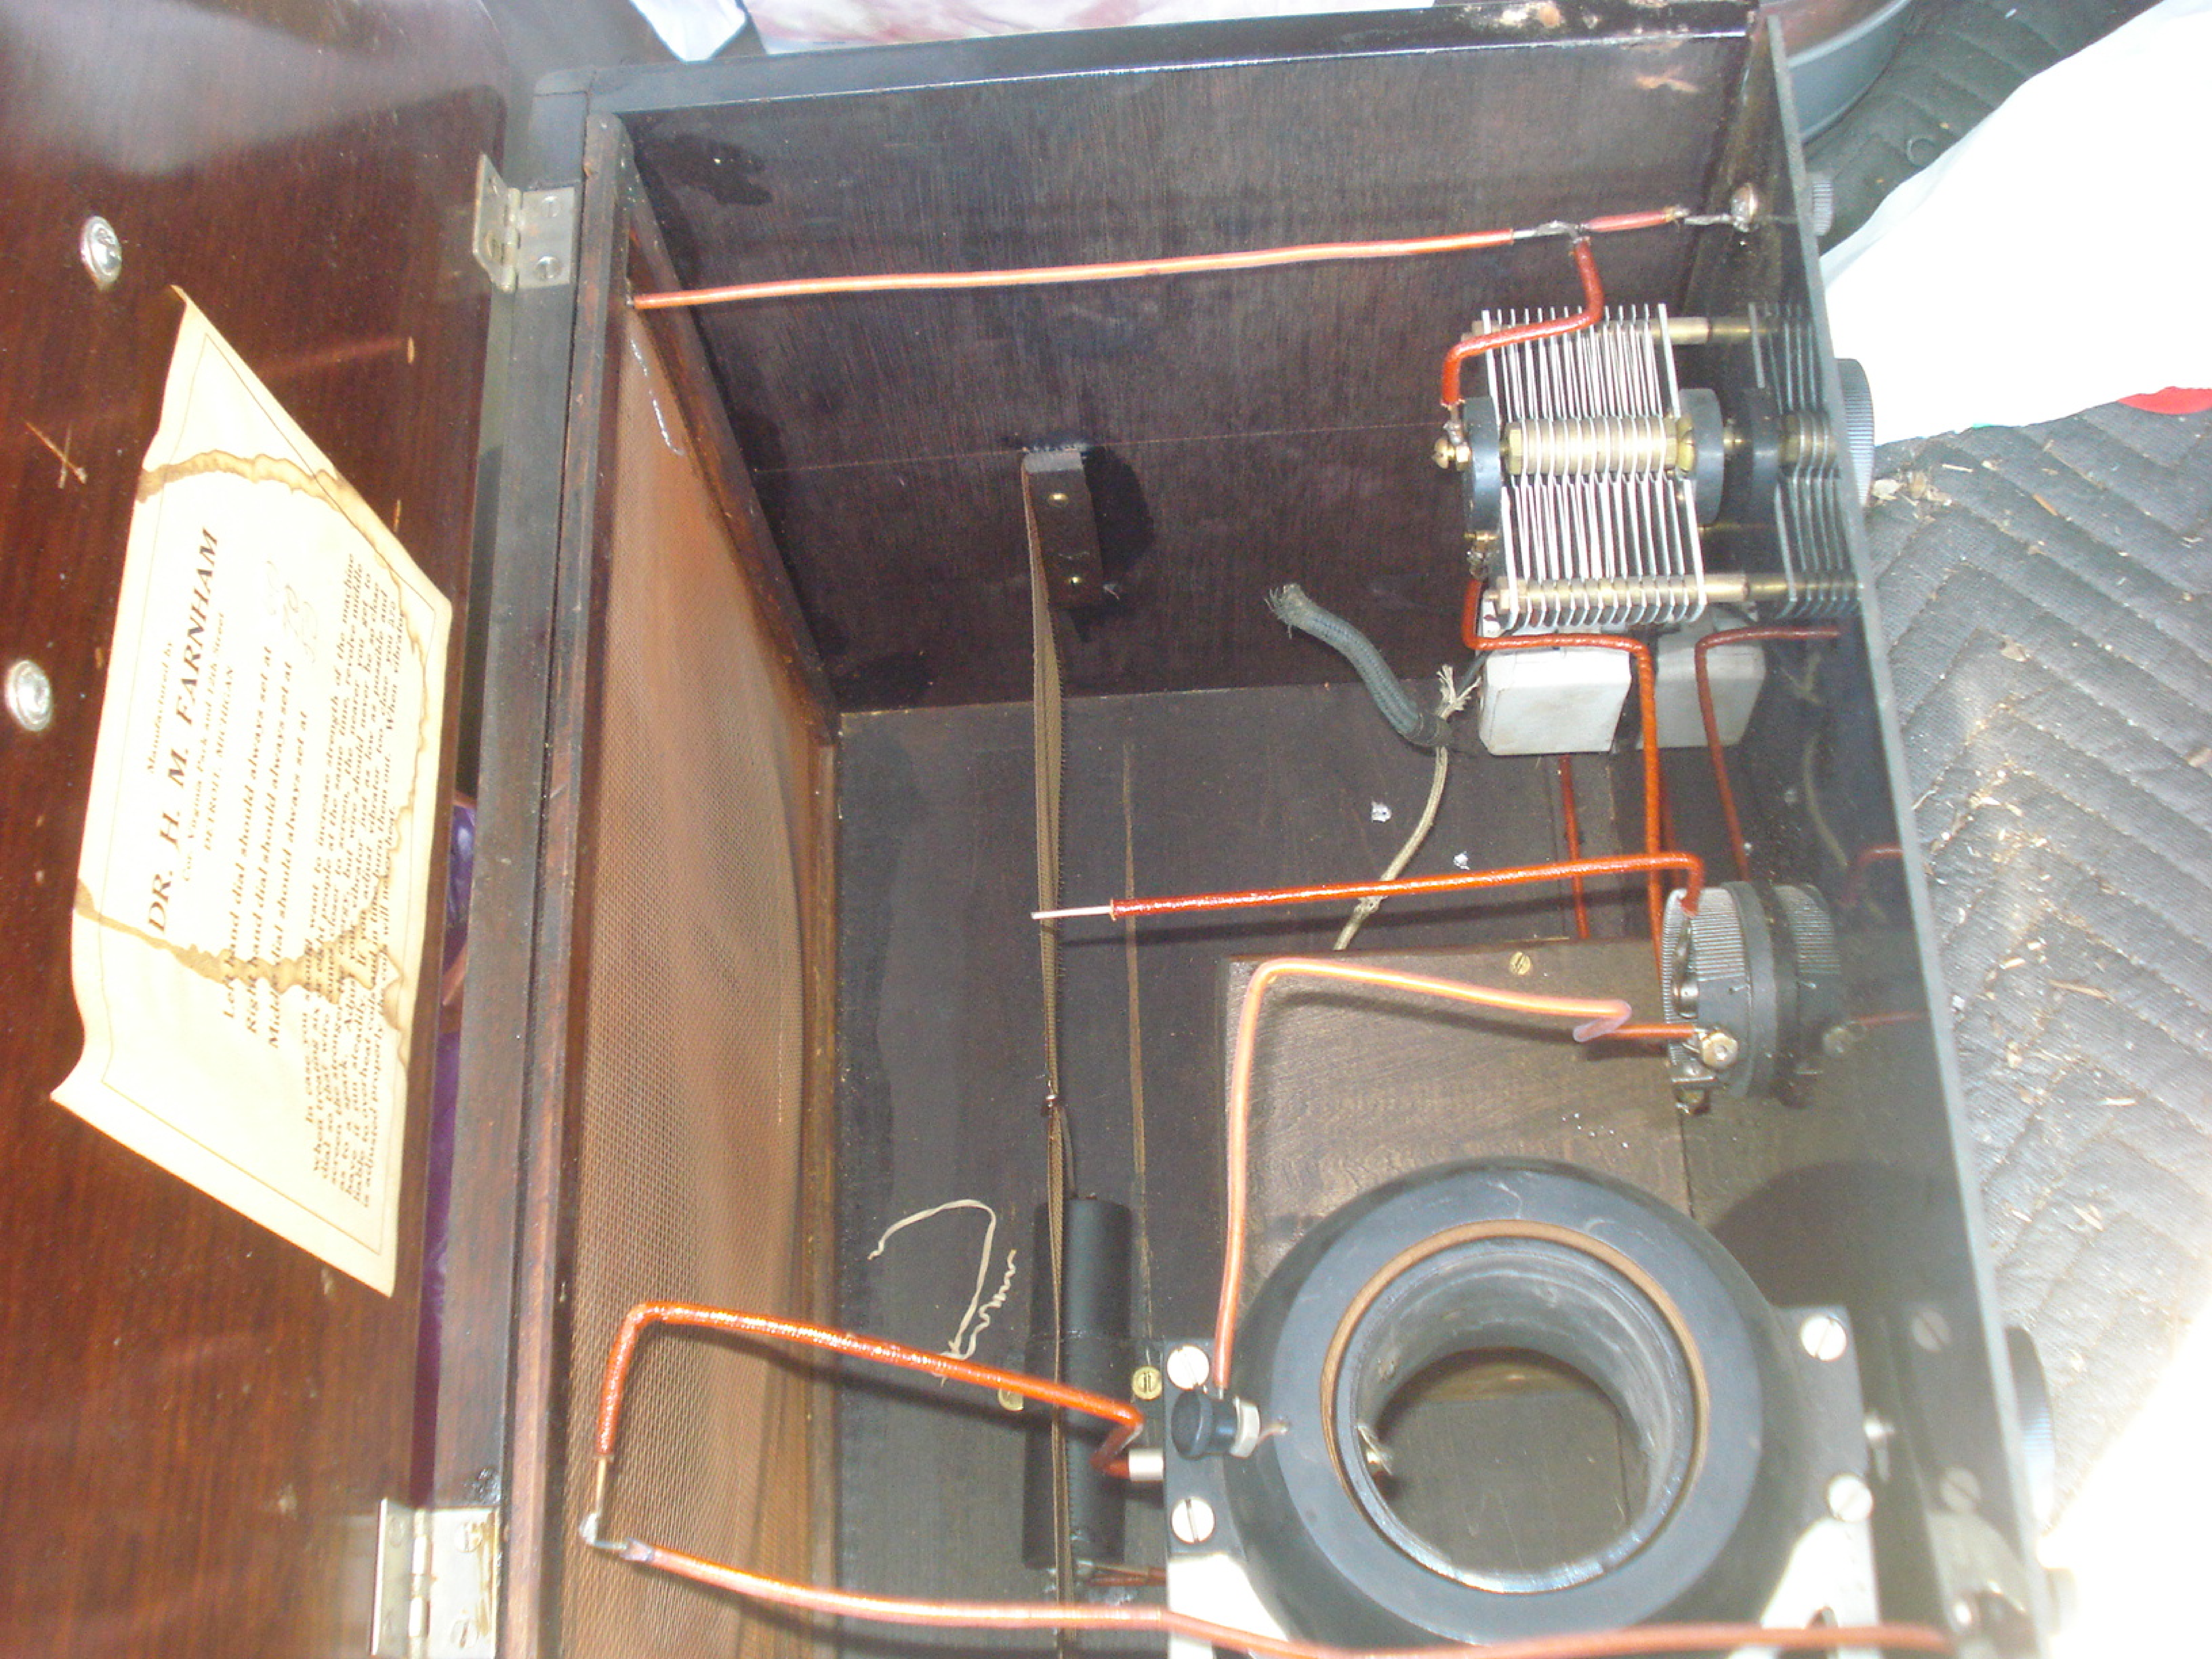
DR. H. M. FARNHAM


case you should want to increase
treating six or eight people at the same time, revolve
so that wire comes closer to screen, the nearer you get to
the stronger the energy, but wire should never be so close
a spark. Adjust your vibrator just as low as possible and
it run steadily. If you adjust vibrator too close you are
to overheat coils and in time burn them out. When vibrator
adjusted properly the coils will never heat




637
6




GRAY DAVIS


DR. HATHAWAY'S
Electro-Magnetic Chair.
1404


1404


Fischer
CHICAGO, ILL.
PAT. APPLD. FOR
TWIN
CARBON
ARC LAMP
VOLTS
110
AMPS.
12
MODEL
M


EL PRODUCTO
I




RAYSUN
THE LIEBEL-FLARSHEIM CO.
CINCINNATI - OHIO
110 VOLTS - 15 AMP.
SERIAL № 2285
1257


1267


BATTLE CREEK
MERCURY SUNARC LAMP
TYPE U 3 MODEL SL 1 NO. 298
MANUFACTURED BY
SANITARIUM EQUIPMENT CO.
BATTLE CREEK, MICH. U.S.A.
PATENT APPLIED FOR
VOLTS 115 AC CYCLES 60 AMPS 14






BRITESUN, INC.
MADE IN U.S.A.
"BRITESUN"
MAJOR
DEEP THERAPY
LAMP
PATENTS APPL. FOR
CHICAGO ELECTRO PHYSIOTHERAPY EQUIPMENT ILLINOIS










1952


EVINRUDE
OUTBOARD MOTORS
Sales-Service



ULTRA SHORT WAVE
RADIOTHERMY
6 METERS 600 WATTS
LARYNGOLOGY GENERATOR
OUTPUT
POWER
FILAMENT
PLATE
POWER CONTROL
PATIENT CIRCUITS
SURGERY
PADS
STEPS
CABLE
SURGERY
FILAMENT
ON
OFF
PLATE
ON
OFF



POWER CONTROL
RESONANCE CONTROL
POWER INDICATOR
FISCHERTHERM
SOLE DISTRIBUTOR,
J. BEEBER CO. NEW YORK,
PHILADELPHIA
LICENSED UNDER U.S. PATENTS
FILAMENT
PLATE
HEAVY DUTY S.W.
SURGERY
INDUCTION CABLE
1
2
3
4
5
6
FISCHERTHERM
SHORT WAVE
J. BEEBER CO. NEW YORK
SOLE DISTRIBUTOR


PILOT
FISCHER CORPORATION
POWER CONTROL
RESONANCE CONTROL
POWER INDICATOR
FISCHERTHERM
4TC-103A 15M. S.W. 104B
SOLE DISTRIBUTOR,
J. BEEBER CO., NEW YORK,
PHILADELPHIA
LICENSED UNDER U.S. PATENTS
HEAVY DUTY S.W.
SURGERY
INDUCTION CABLE
FILAMENT
PLATE



FISCHERTHERM
SHORT WAVE
MINUTES
J. BEEBER CO. NEW YORK
SOLE DISTRIBUTOR




Fischer
CHICAGO, ILL.
PAT. APPLS. FOR
TWIN CARBON
ARC LAMP
VOLTS
110
AMPS.
12
MODEL
M

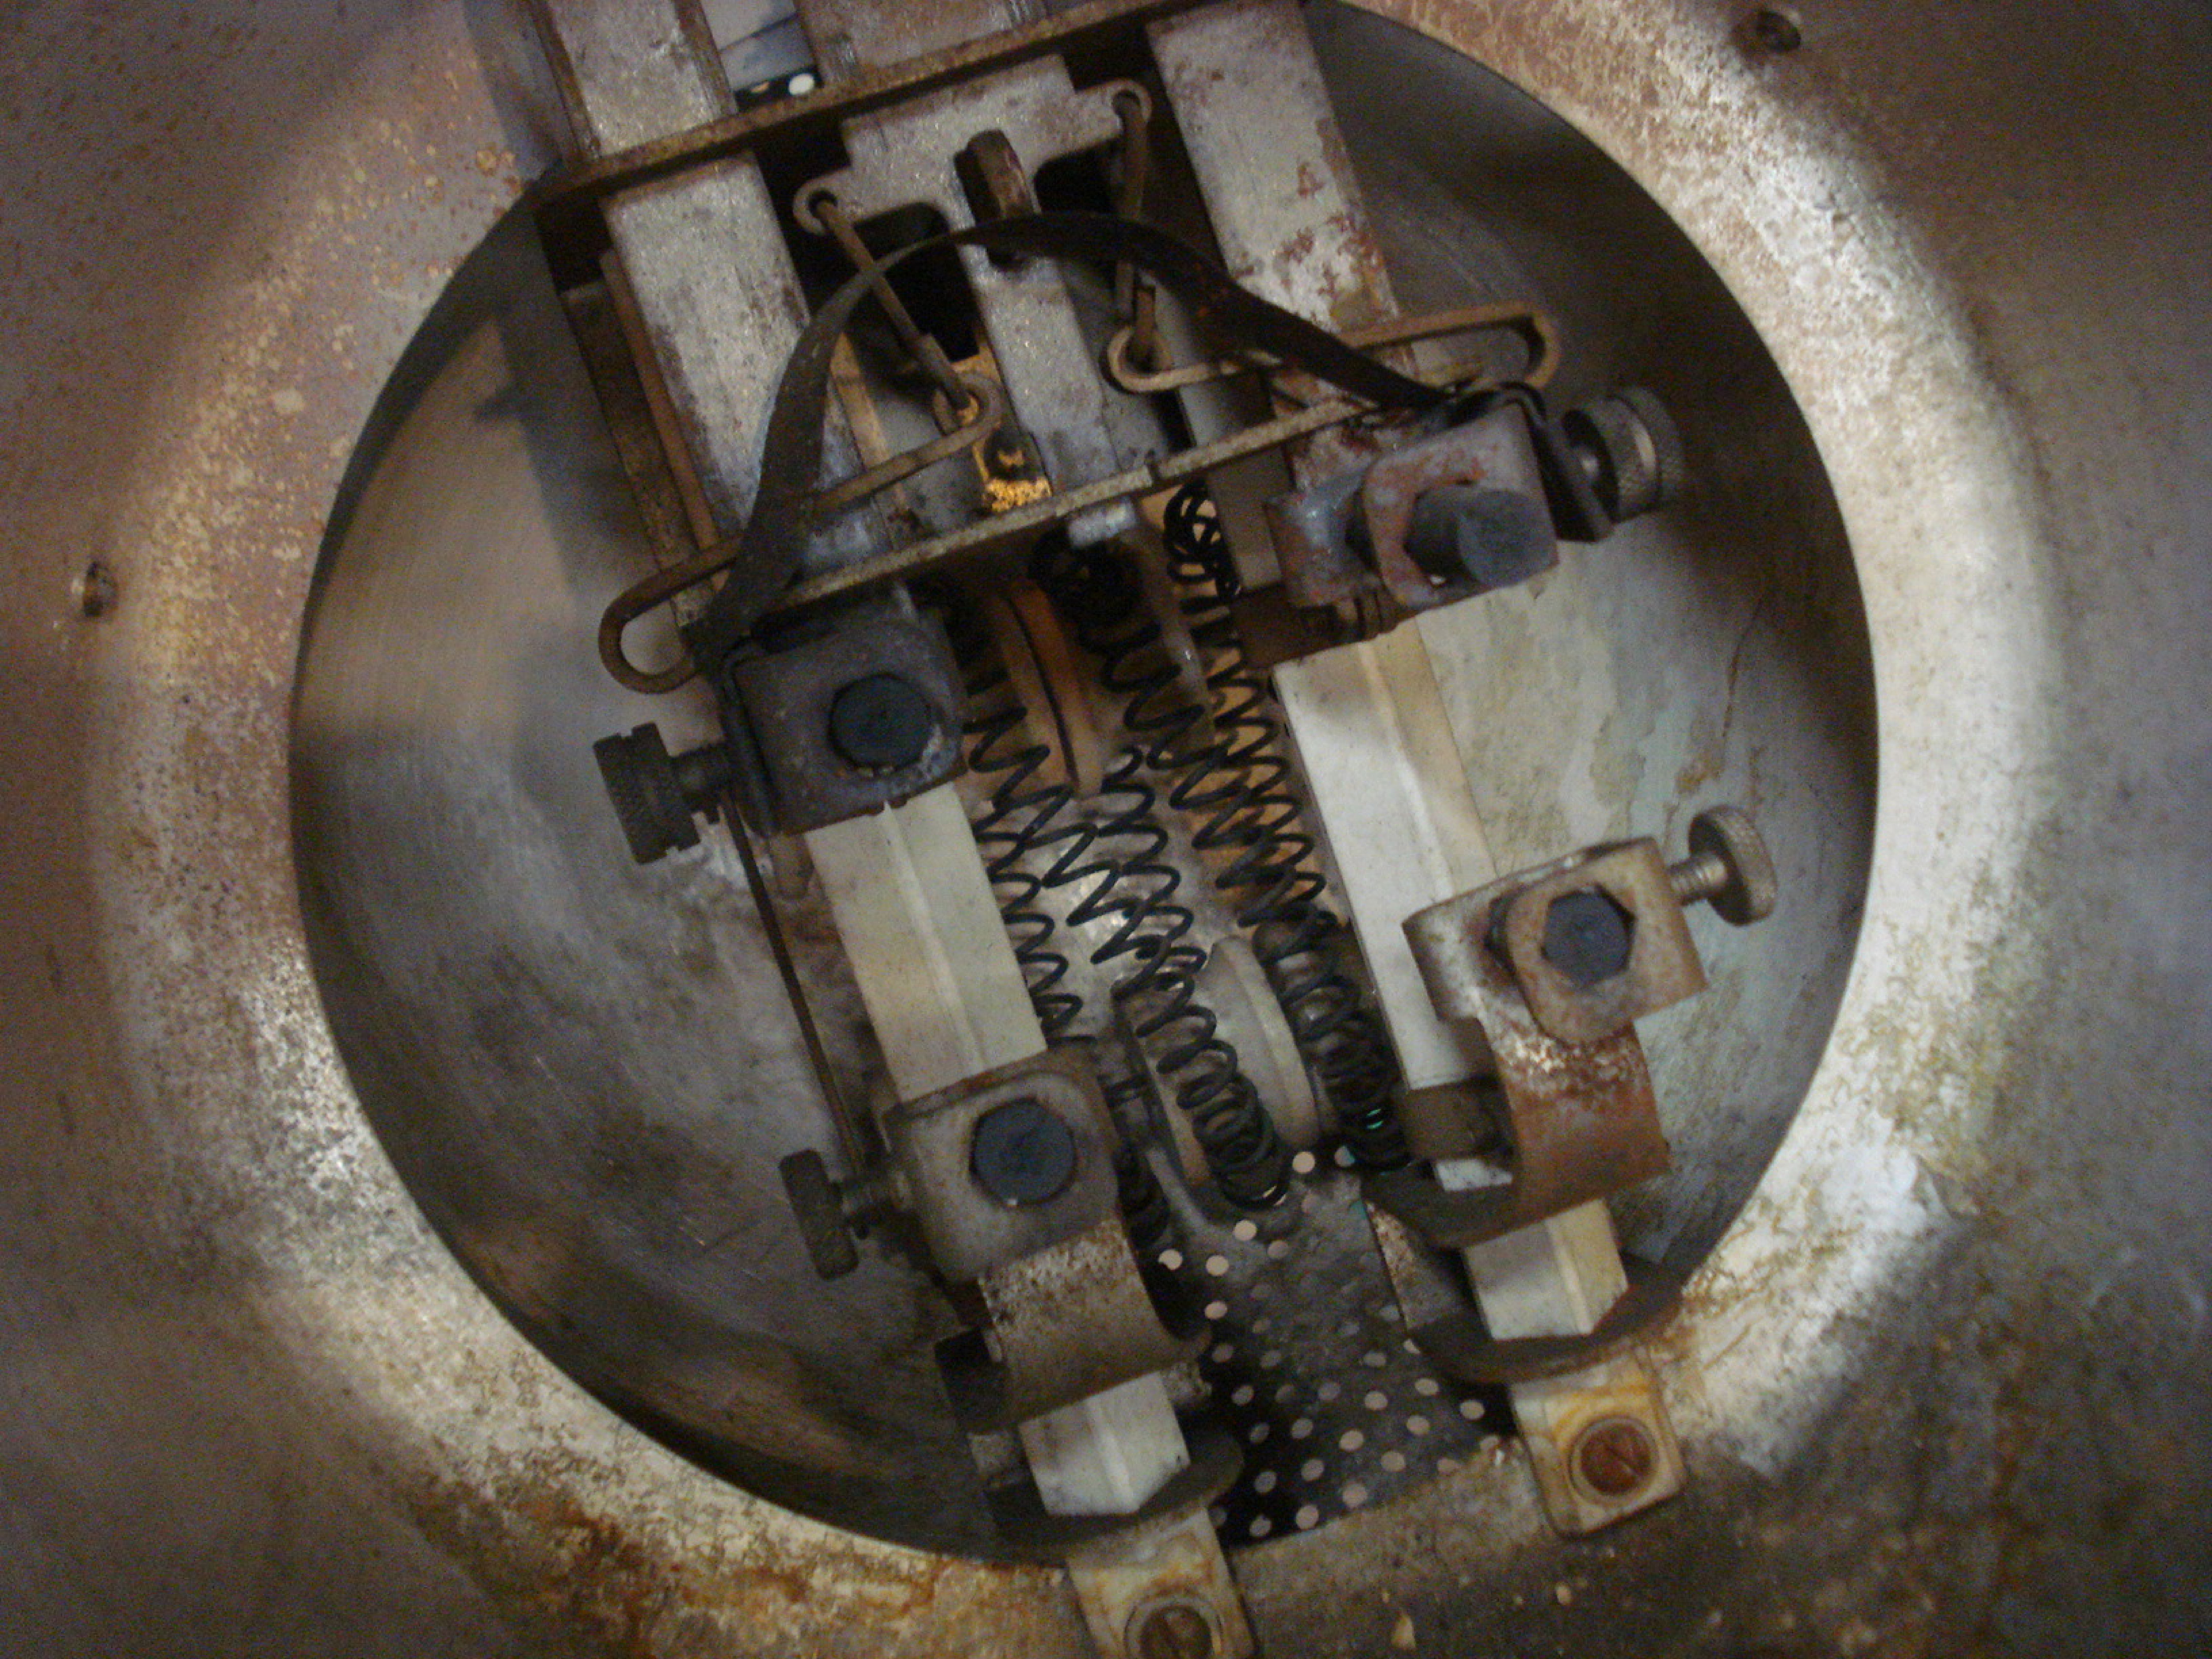


1871

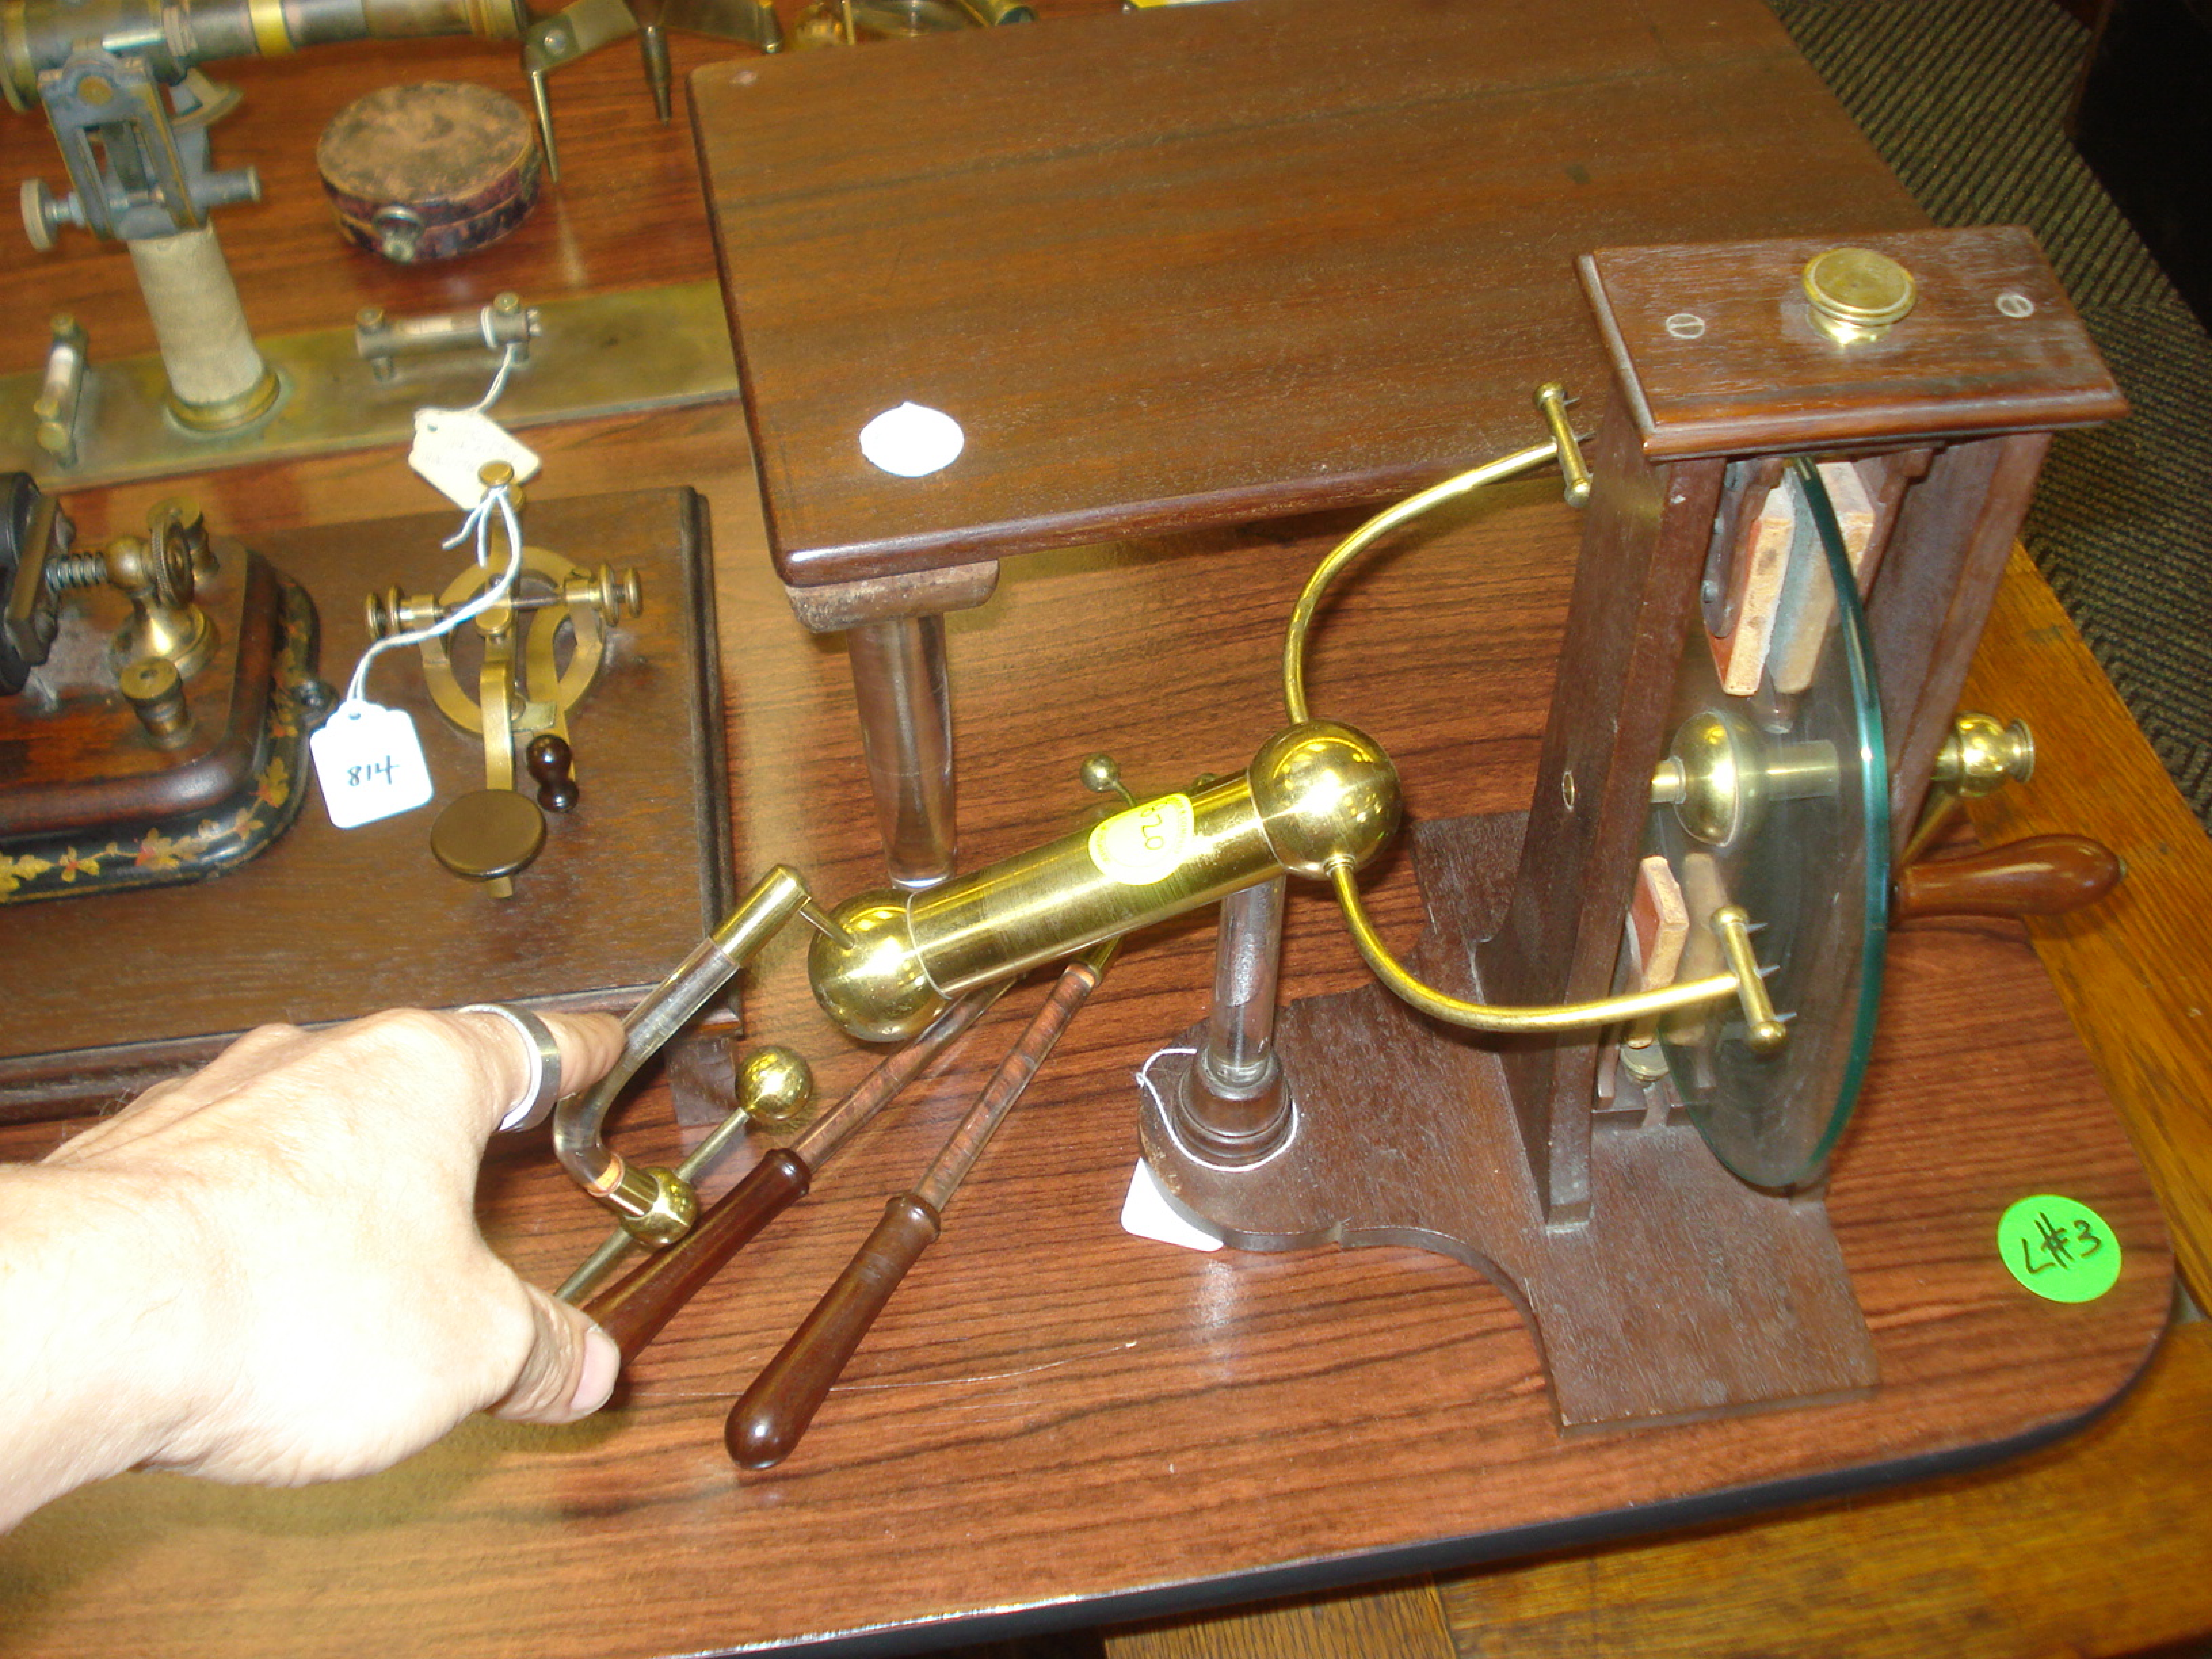
814
L#3




MAKERS






W & S. Jones
N° 30 Holborn
London




















BENJ. PIKE JR.
294 BROADWAY.
N.Y.

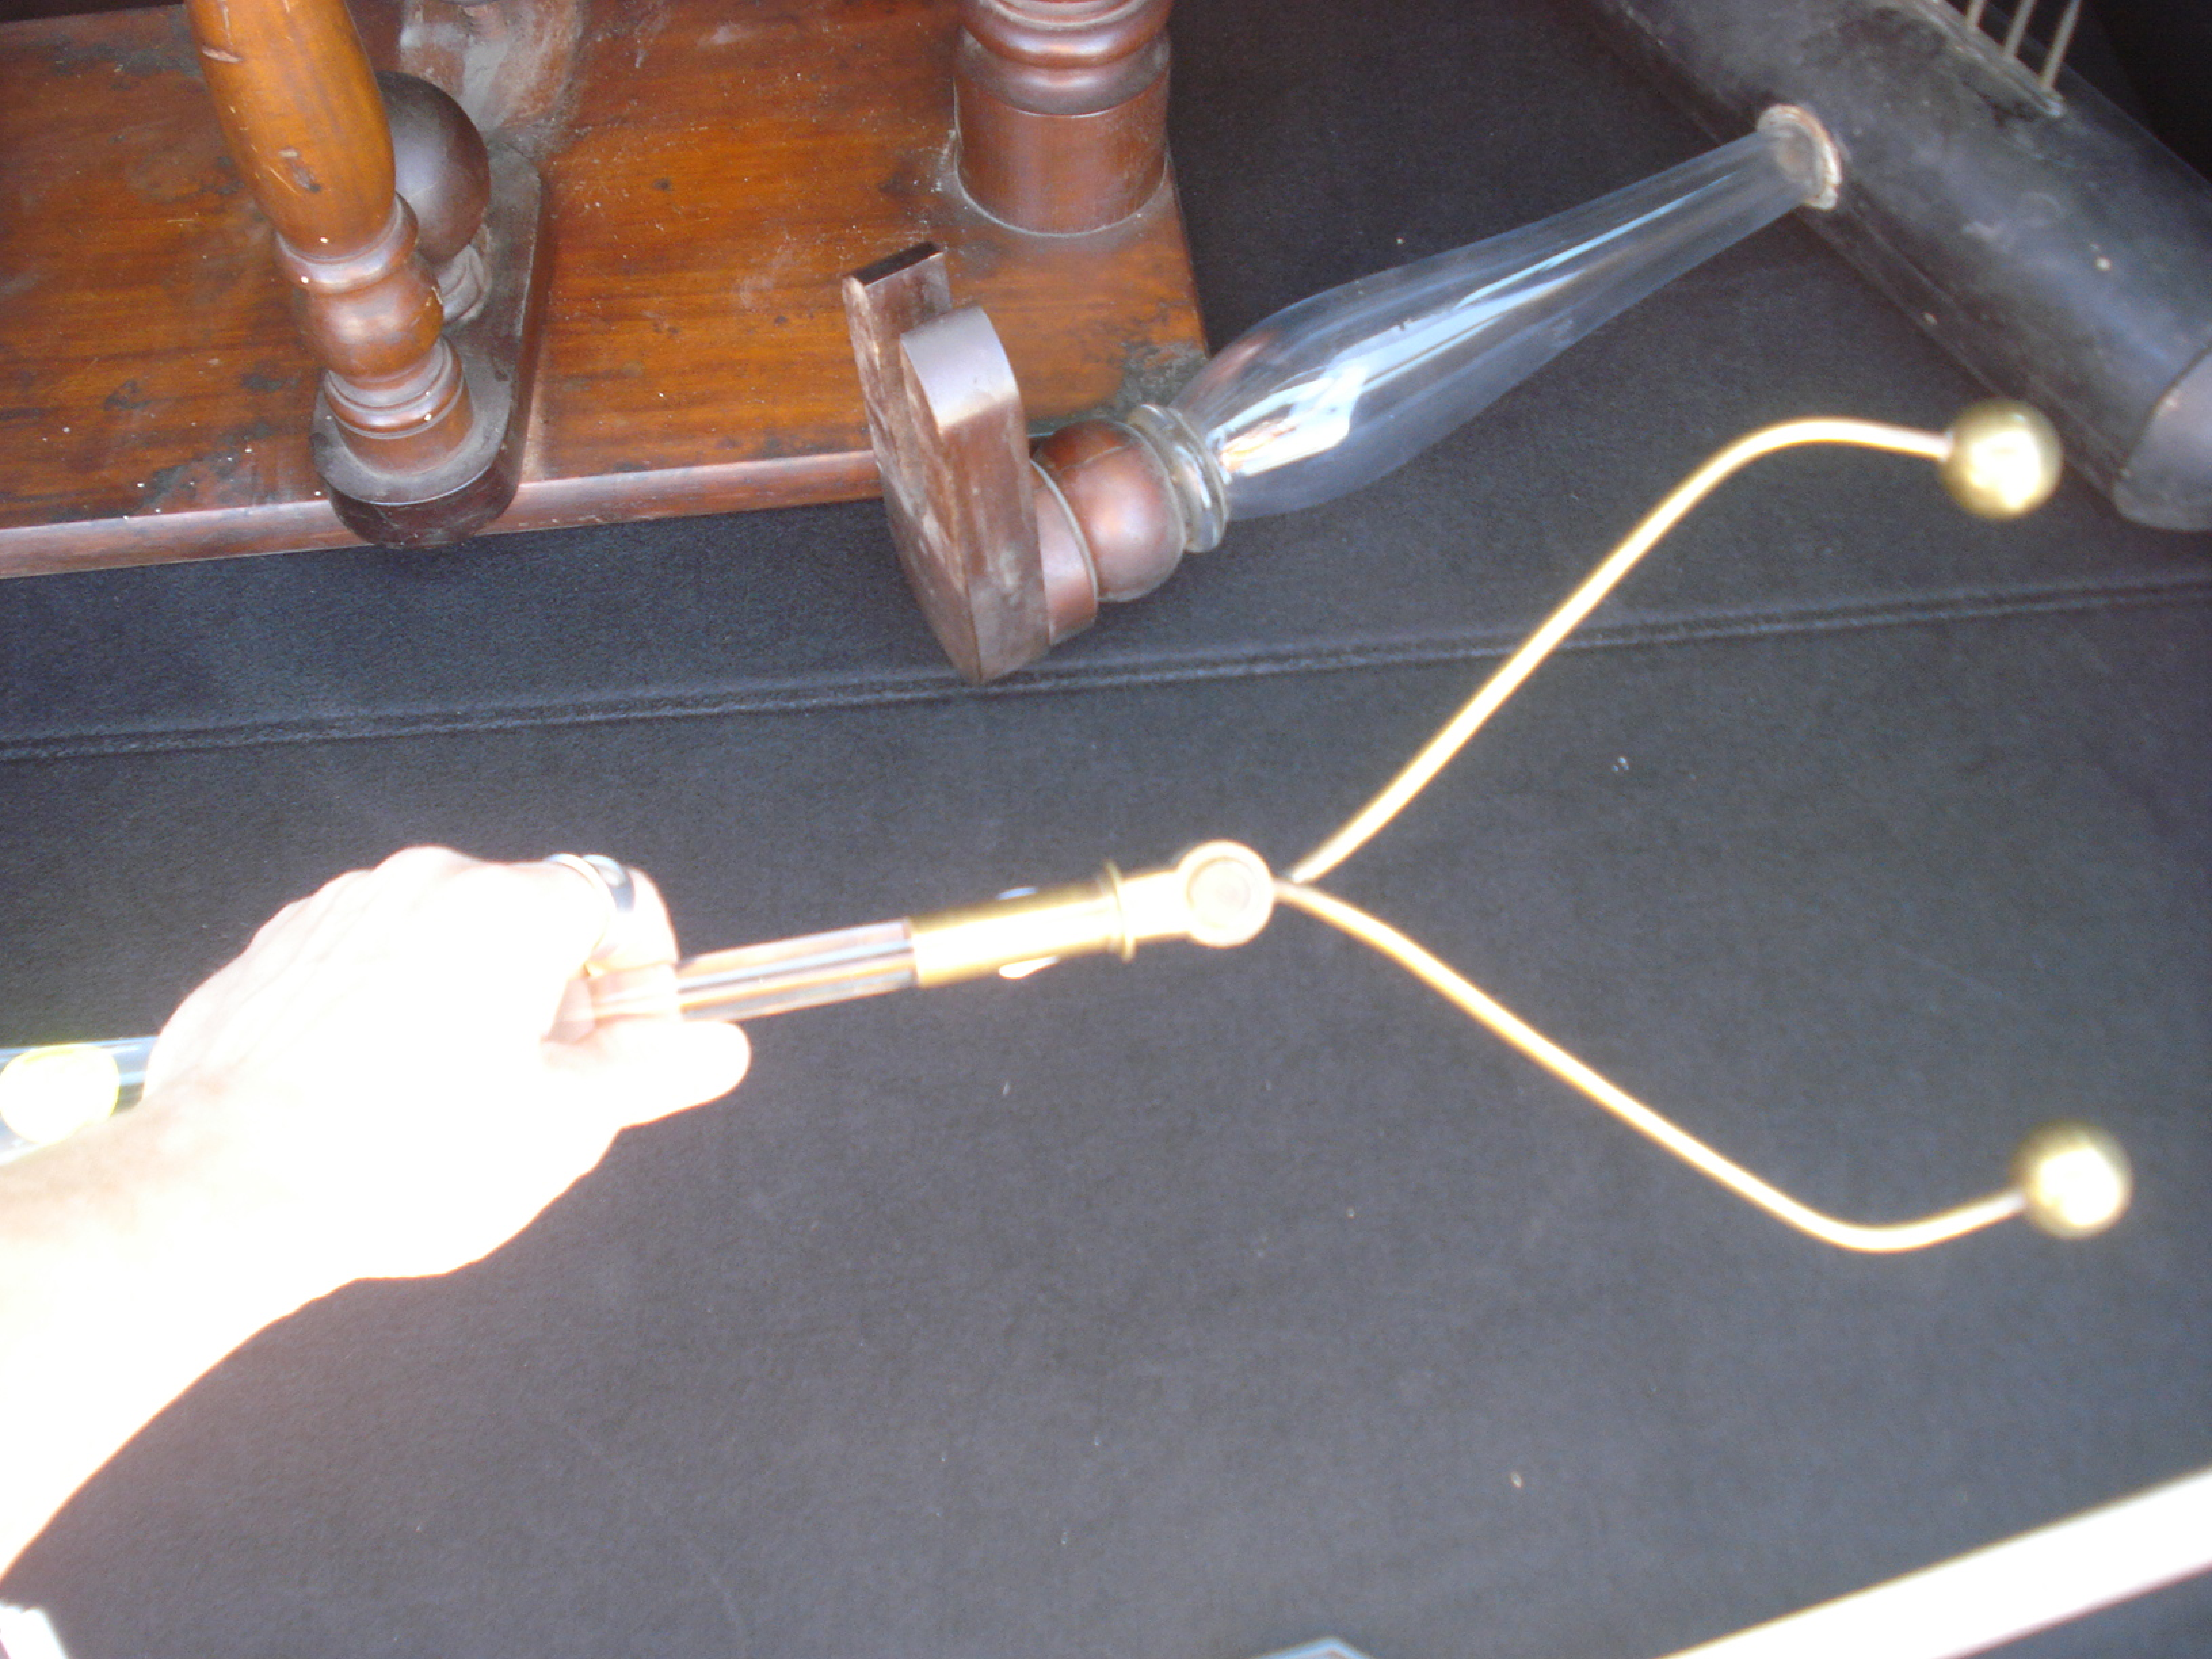

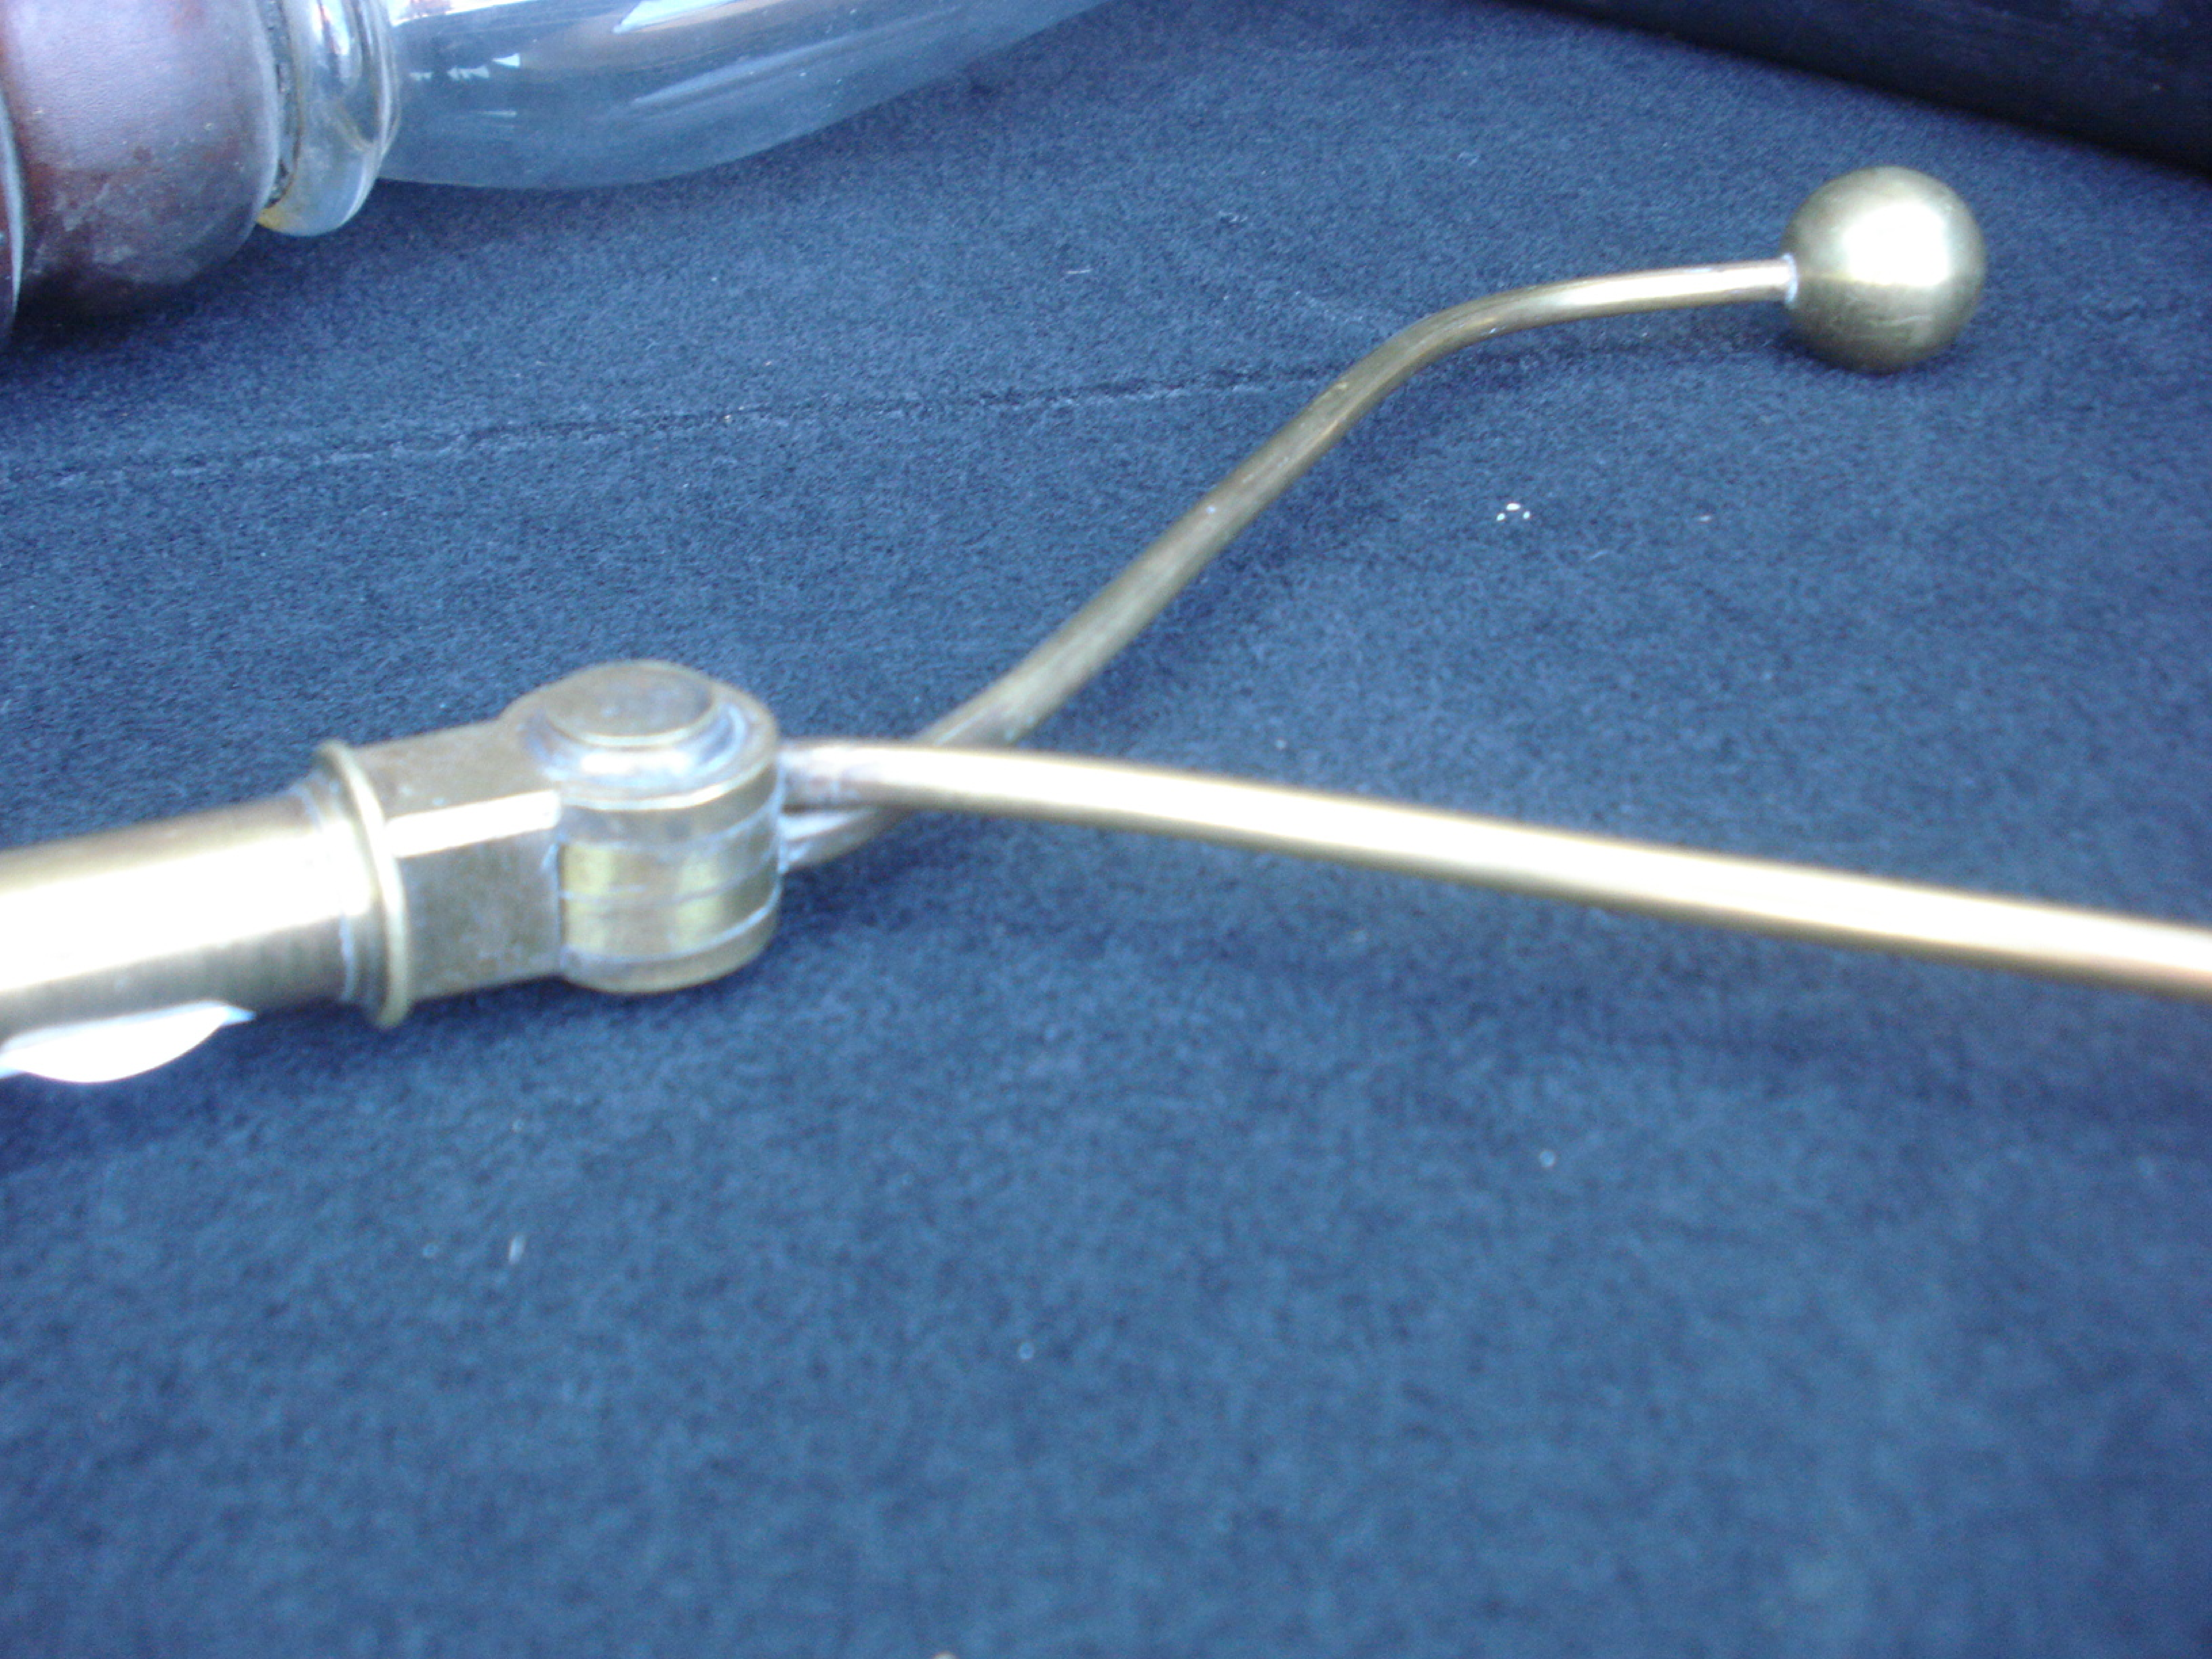



















NEWARK
NEW JERSEY






LPINE SUN LAM
LUXOR MODEL
ANOVIA CHEMICAL & MFG. CO. NEWARK, N.J.

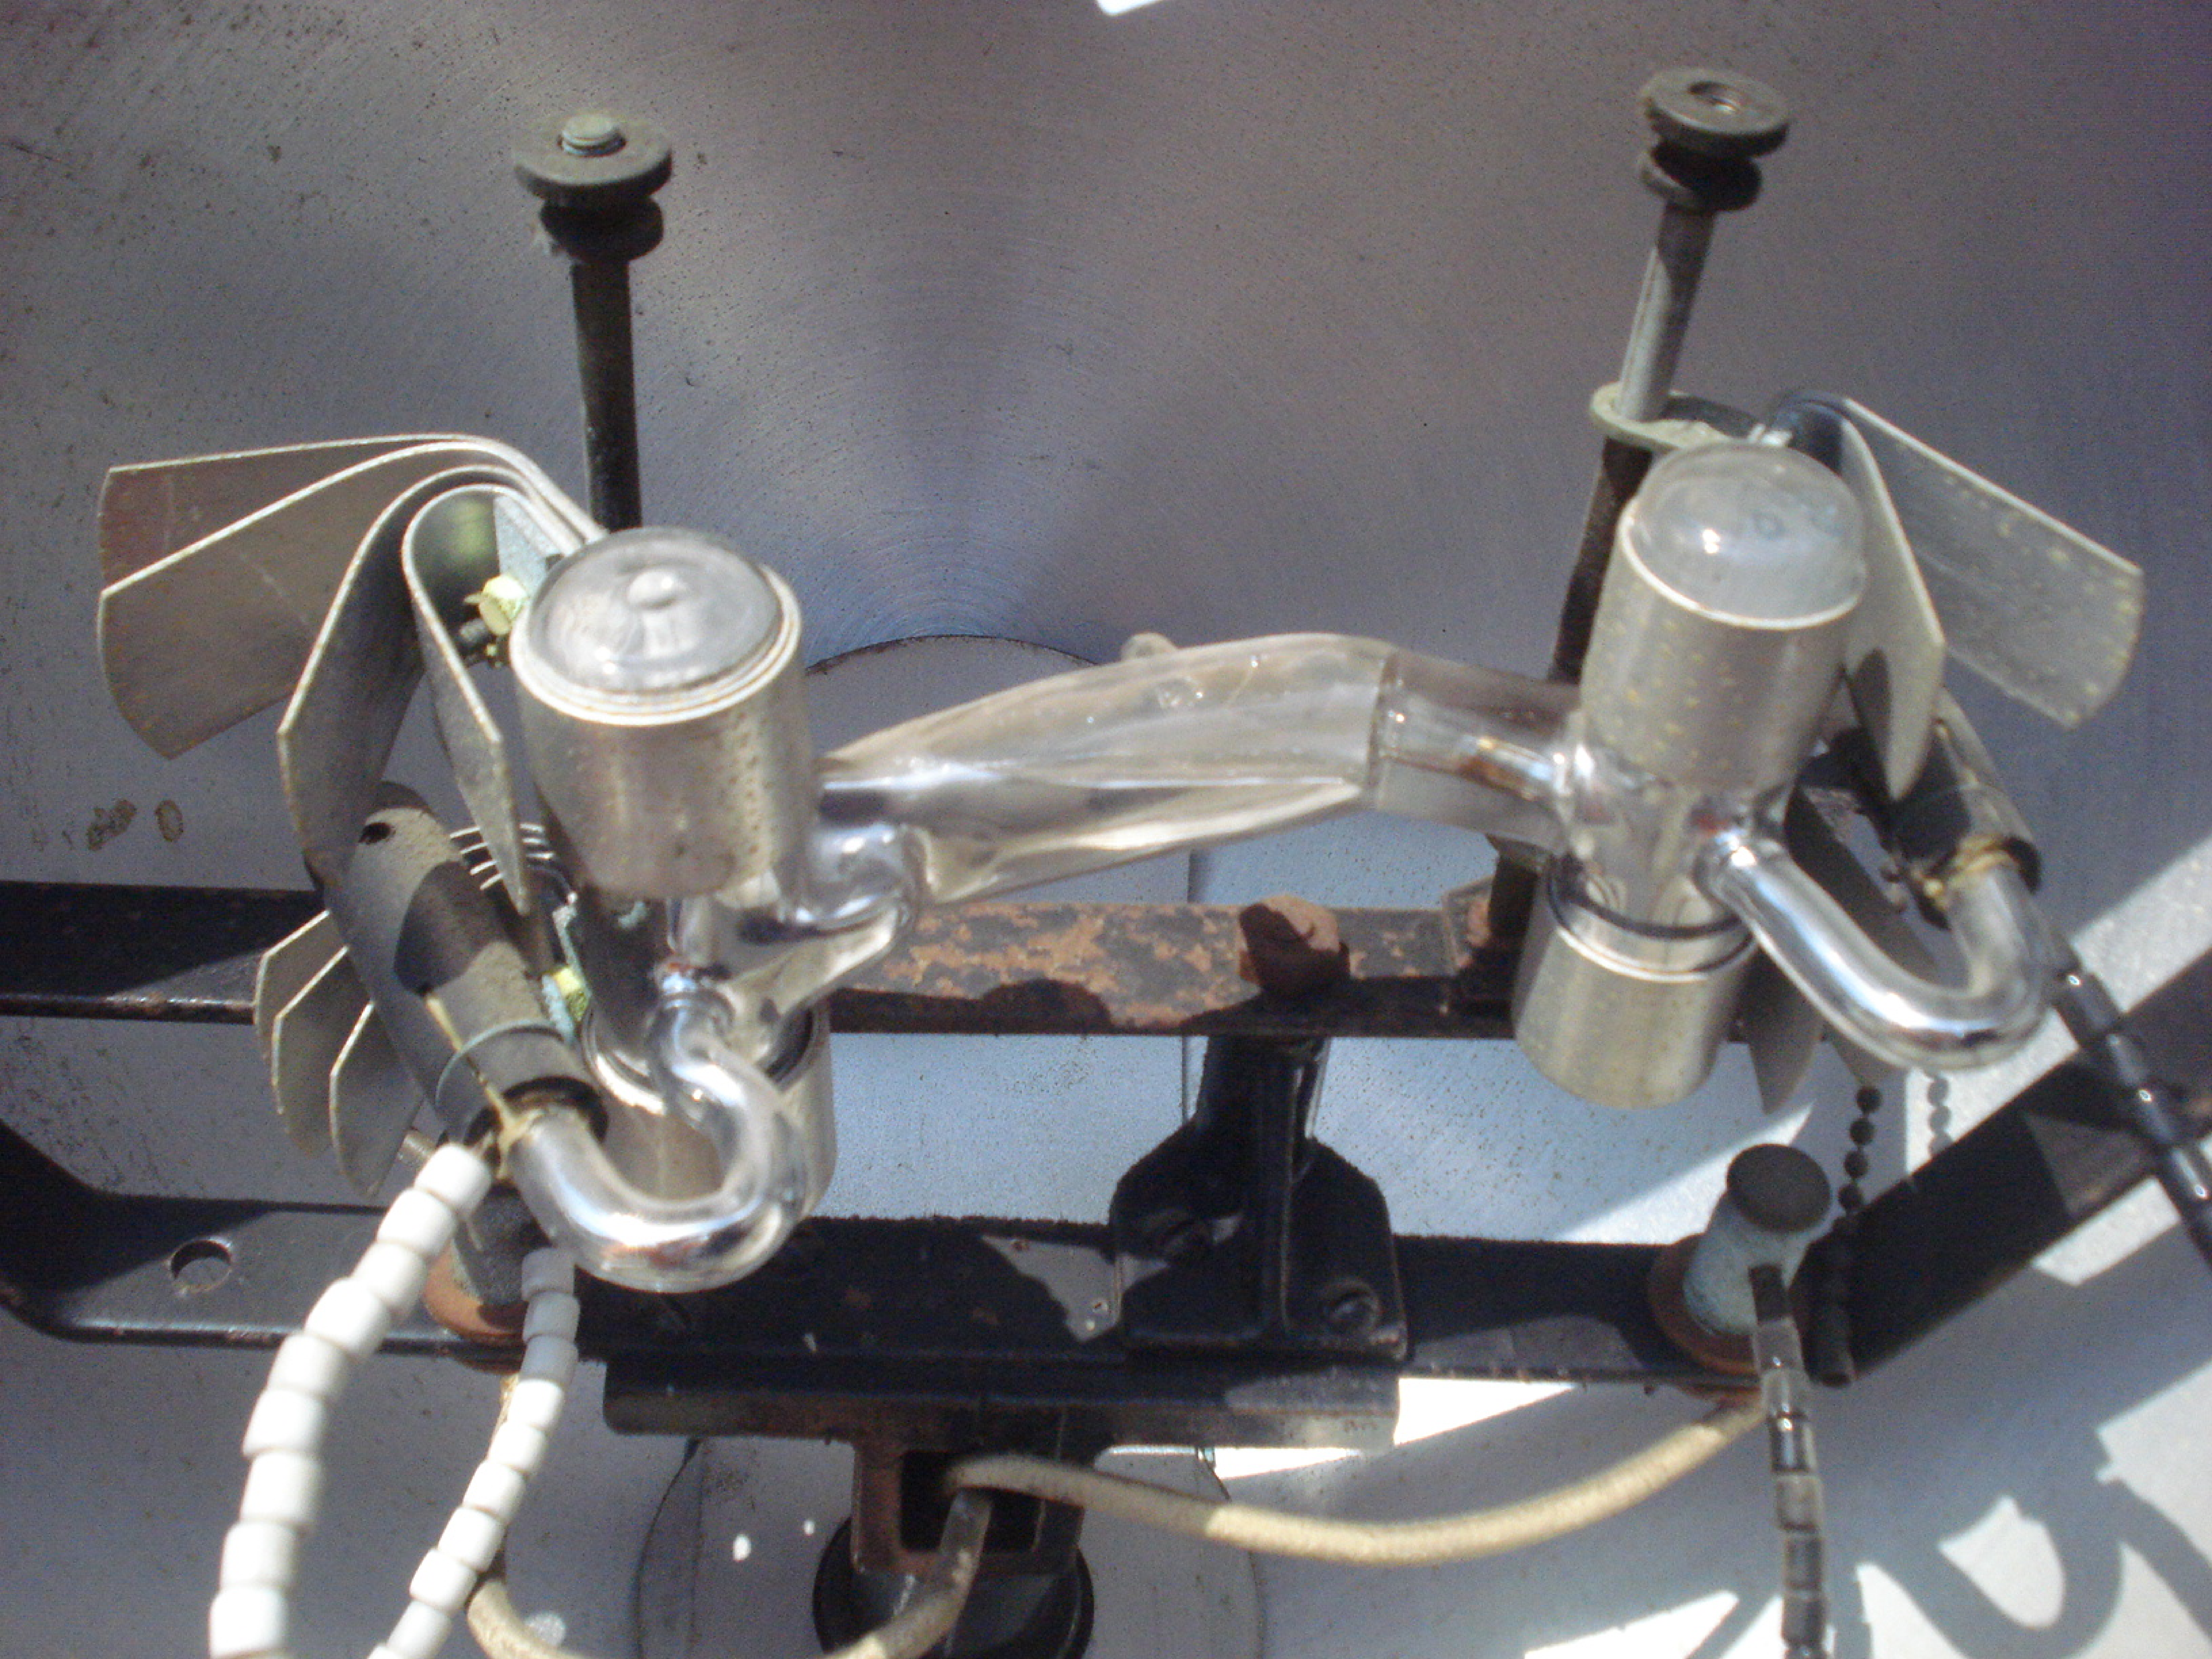




WASH
OFF ARC TUBE
WITH ALCOHOL


TEAM


PATENTS




Campbell


NON-SMOKING ROOM
Thank You For Not Smoking
120V, 60Hz, 11Amps
Max. Combined
CAMPBELL HIGH FREQUENCY COIL
CAMPBELL BRO'S, LYNN, MASS.


HIGH FREQUENCY COIL
4 CYCLES 60 No 367


CAMPBELL HIGH FREQUENCY COIL
VOLTS 110 AMP. 4 CYCLES 60 No 367
CAMPBELL BRO'S. LYNN. MASS.


CAMPBELL HIGH FREQUENCY COIL
VOLTS 110 AMP. 4 CYCLES 60 No 367
CAMPBELL BRO'S, LYNN. MASS.


638



GROGAN & COMPANY
AUCTIONEERS
638
CAMPBELL
VOLTS 110 AMP
CAMPBELL


CAMPBELL ELECTRIC CO
LYNN, MASS


CAMPBELL HIGH FREQUENCY COIL
VOLTS 110 AMP. 4 CYCLES 60 No 367
CAMPBELL BRO'S, LYNN. MASS.



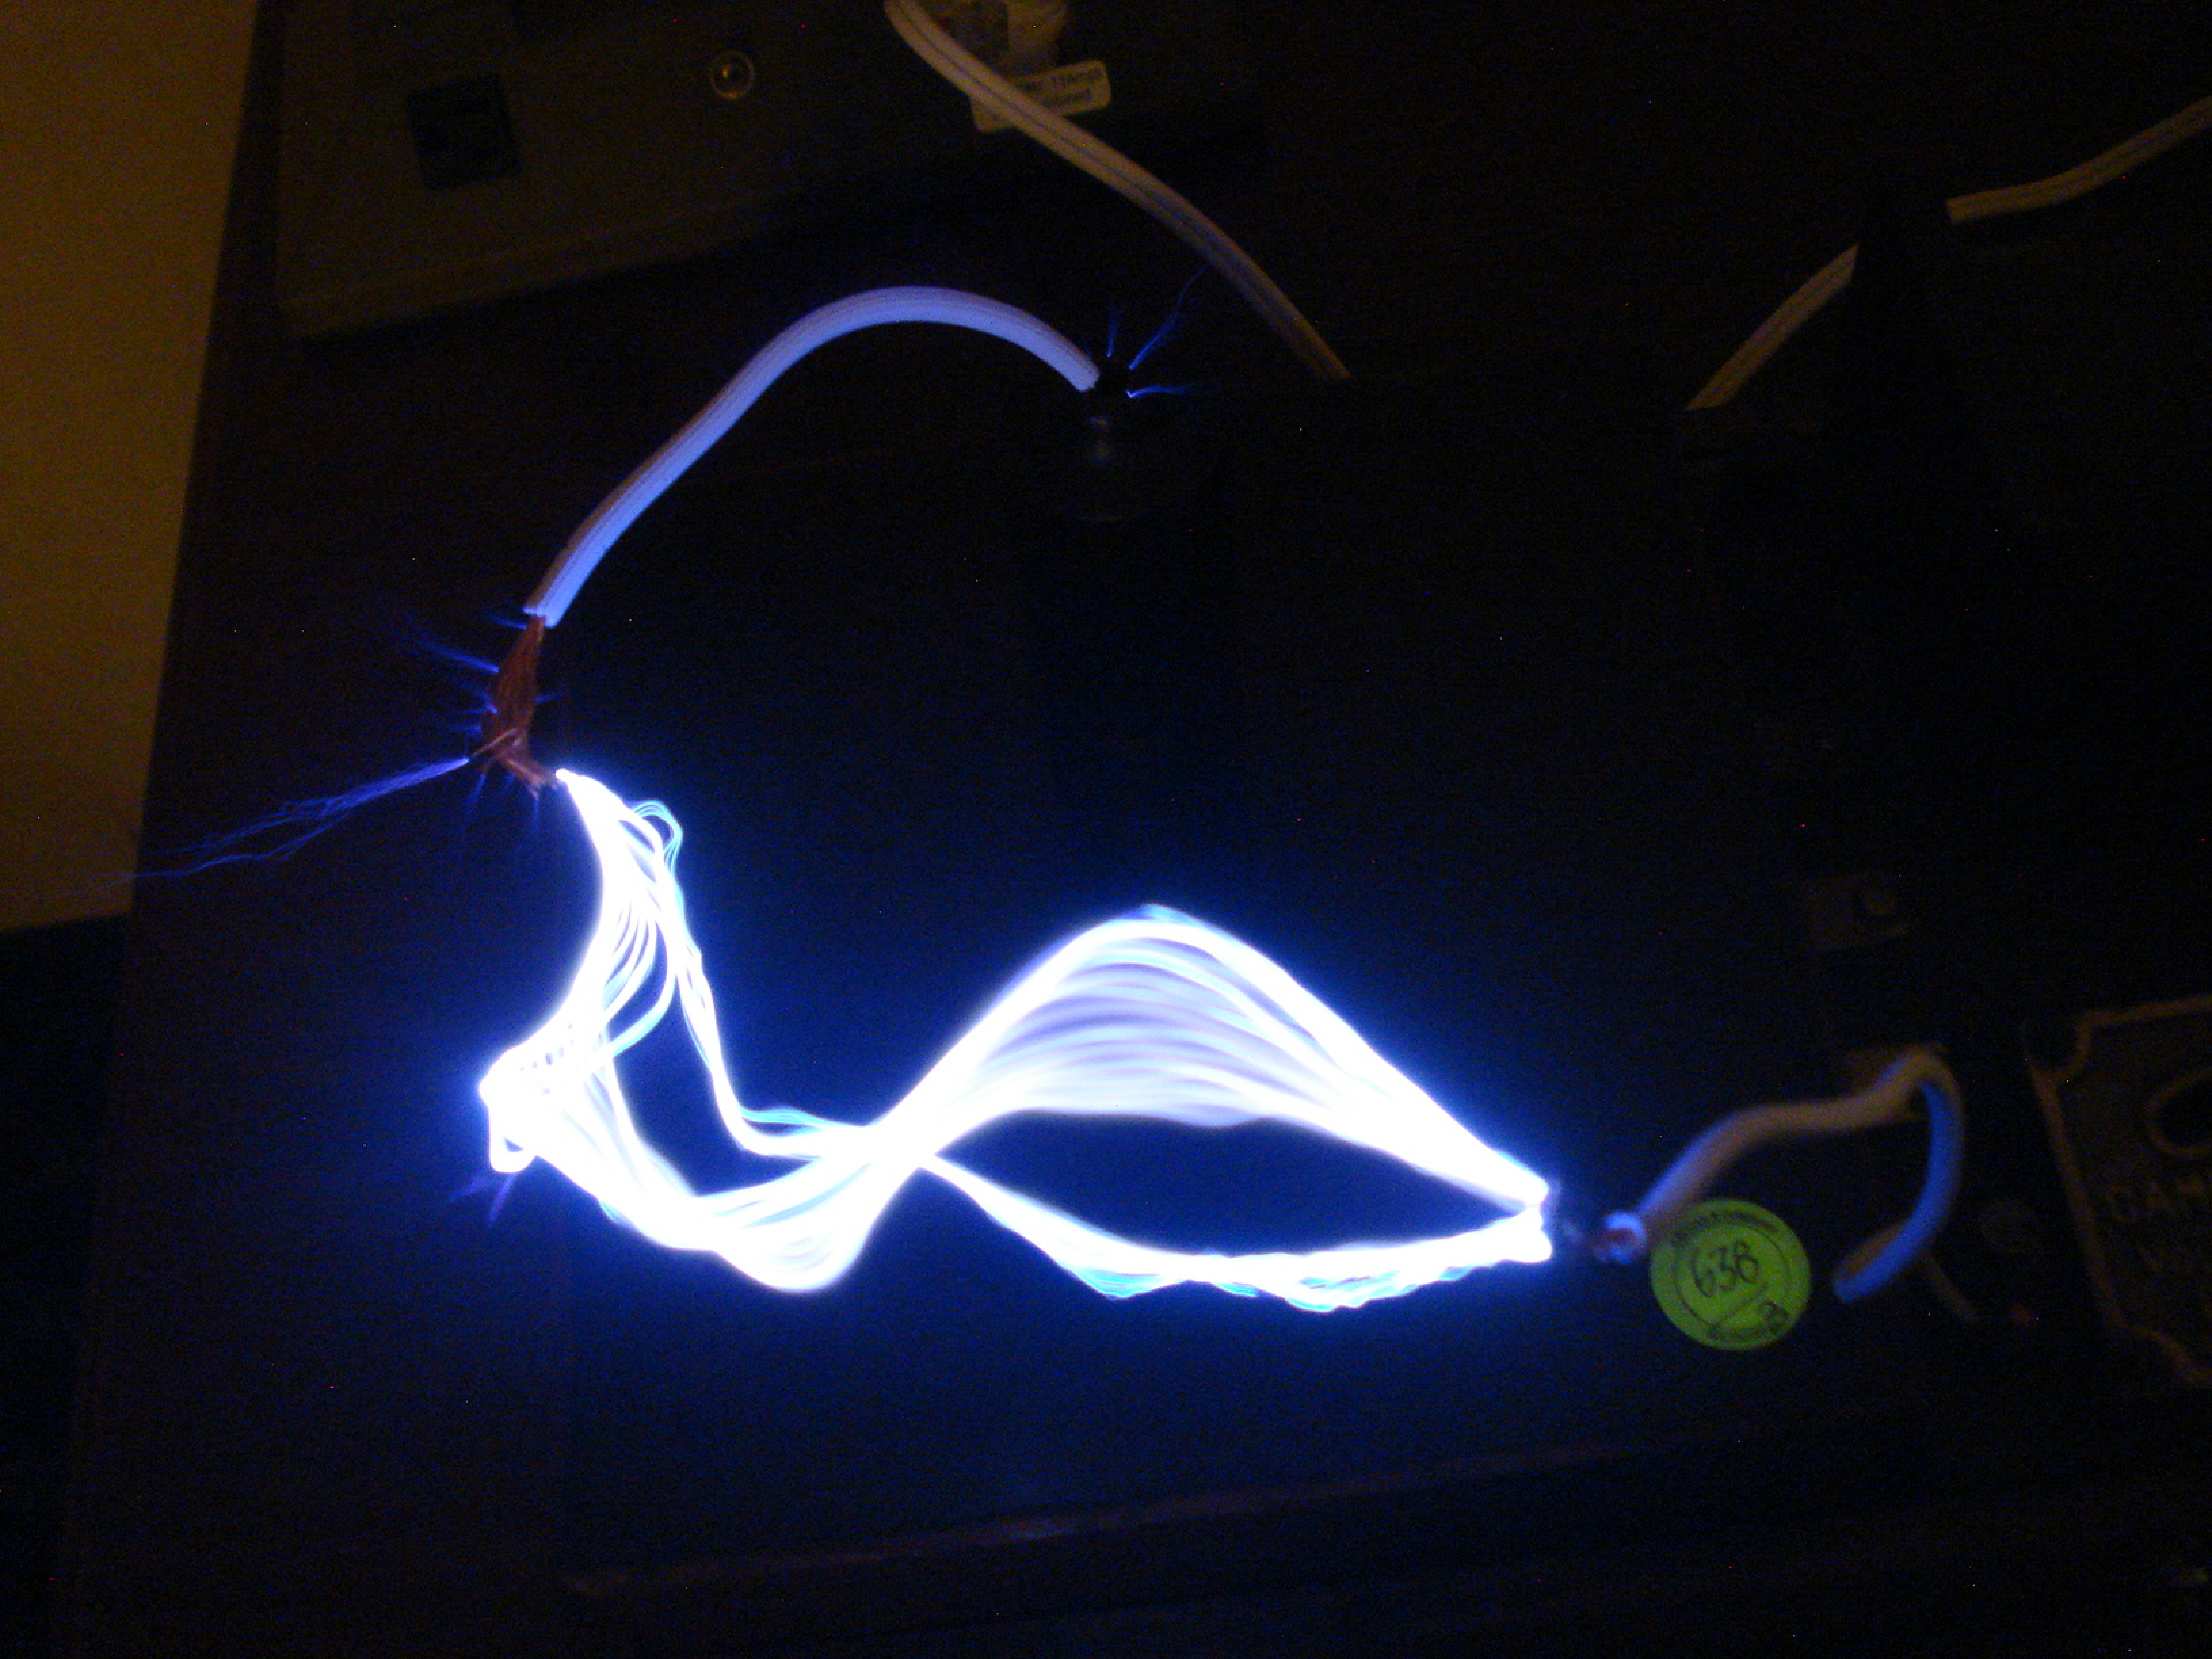


638





Campbell



CAMPBELL HIGH FREQUENCY COIL
VOLTS 110 AMP. 4 CYCLES 60
CAMPBELL BRO'S. LYNN, MASS.




CAMPBELL HIGH FREQUENCY COIL
VOLTS 110 AMP. 4 CYCLES 60 No 367
CAMPBELL BRO'S. LYNN. MASS.

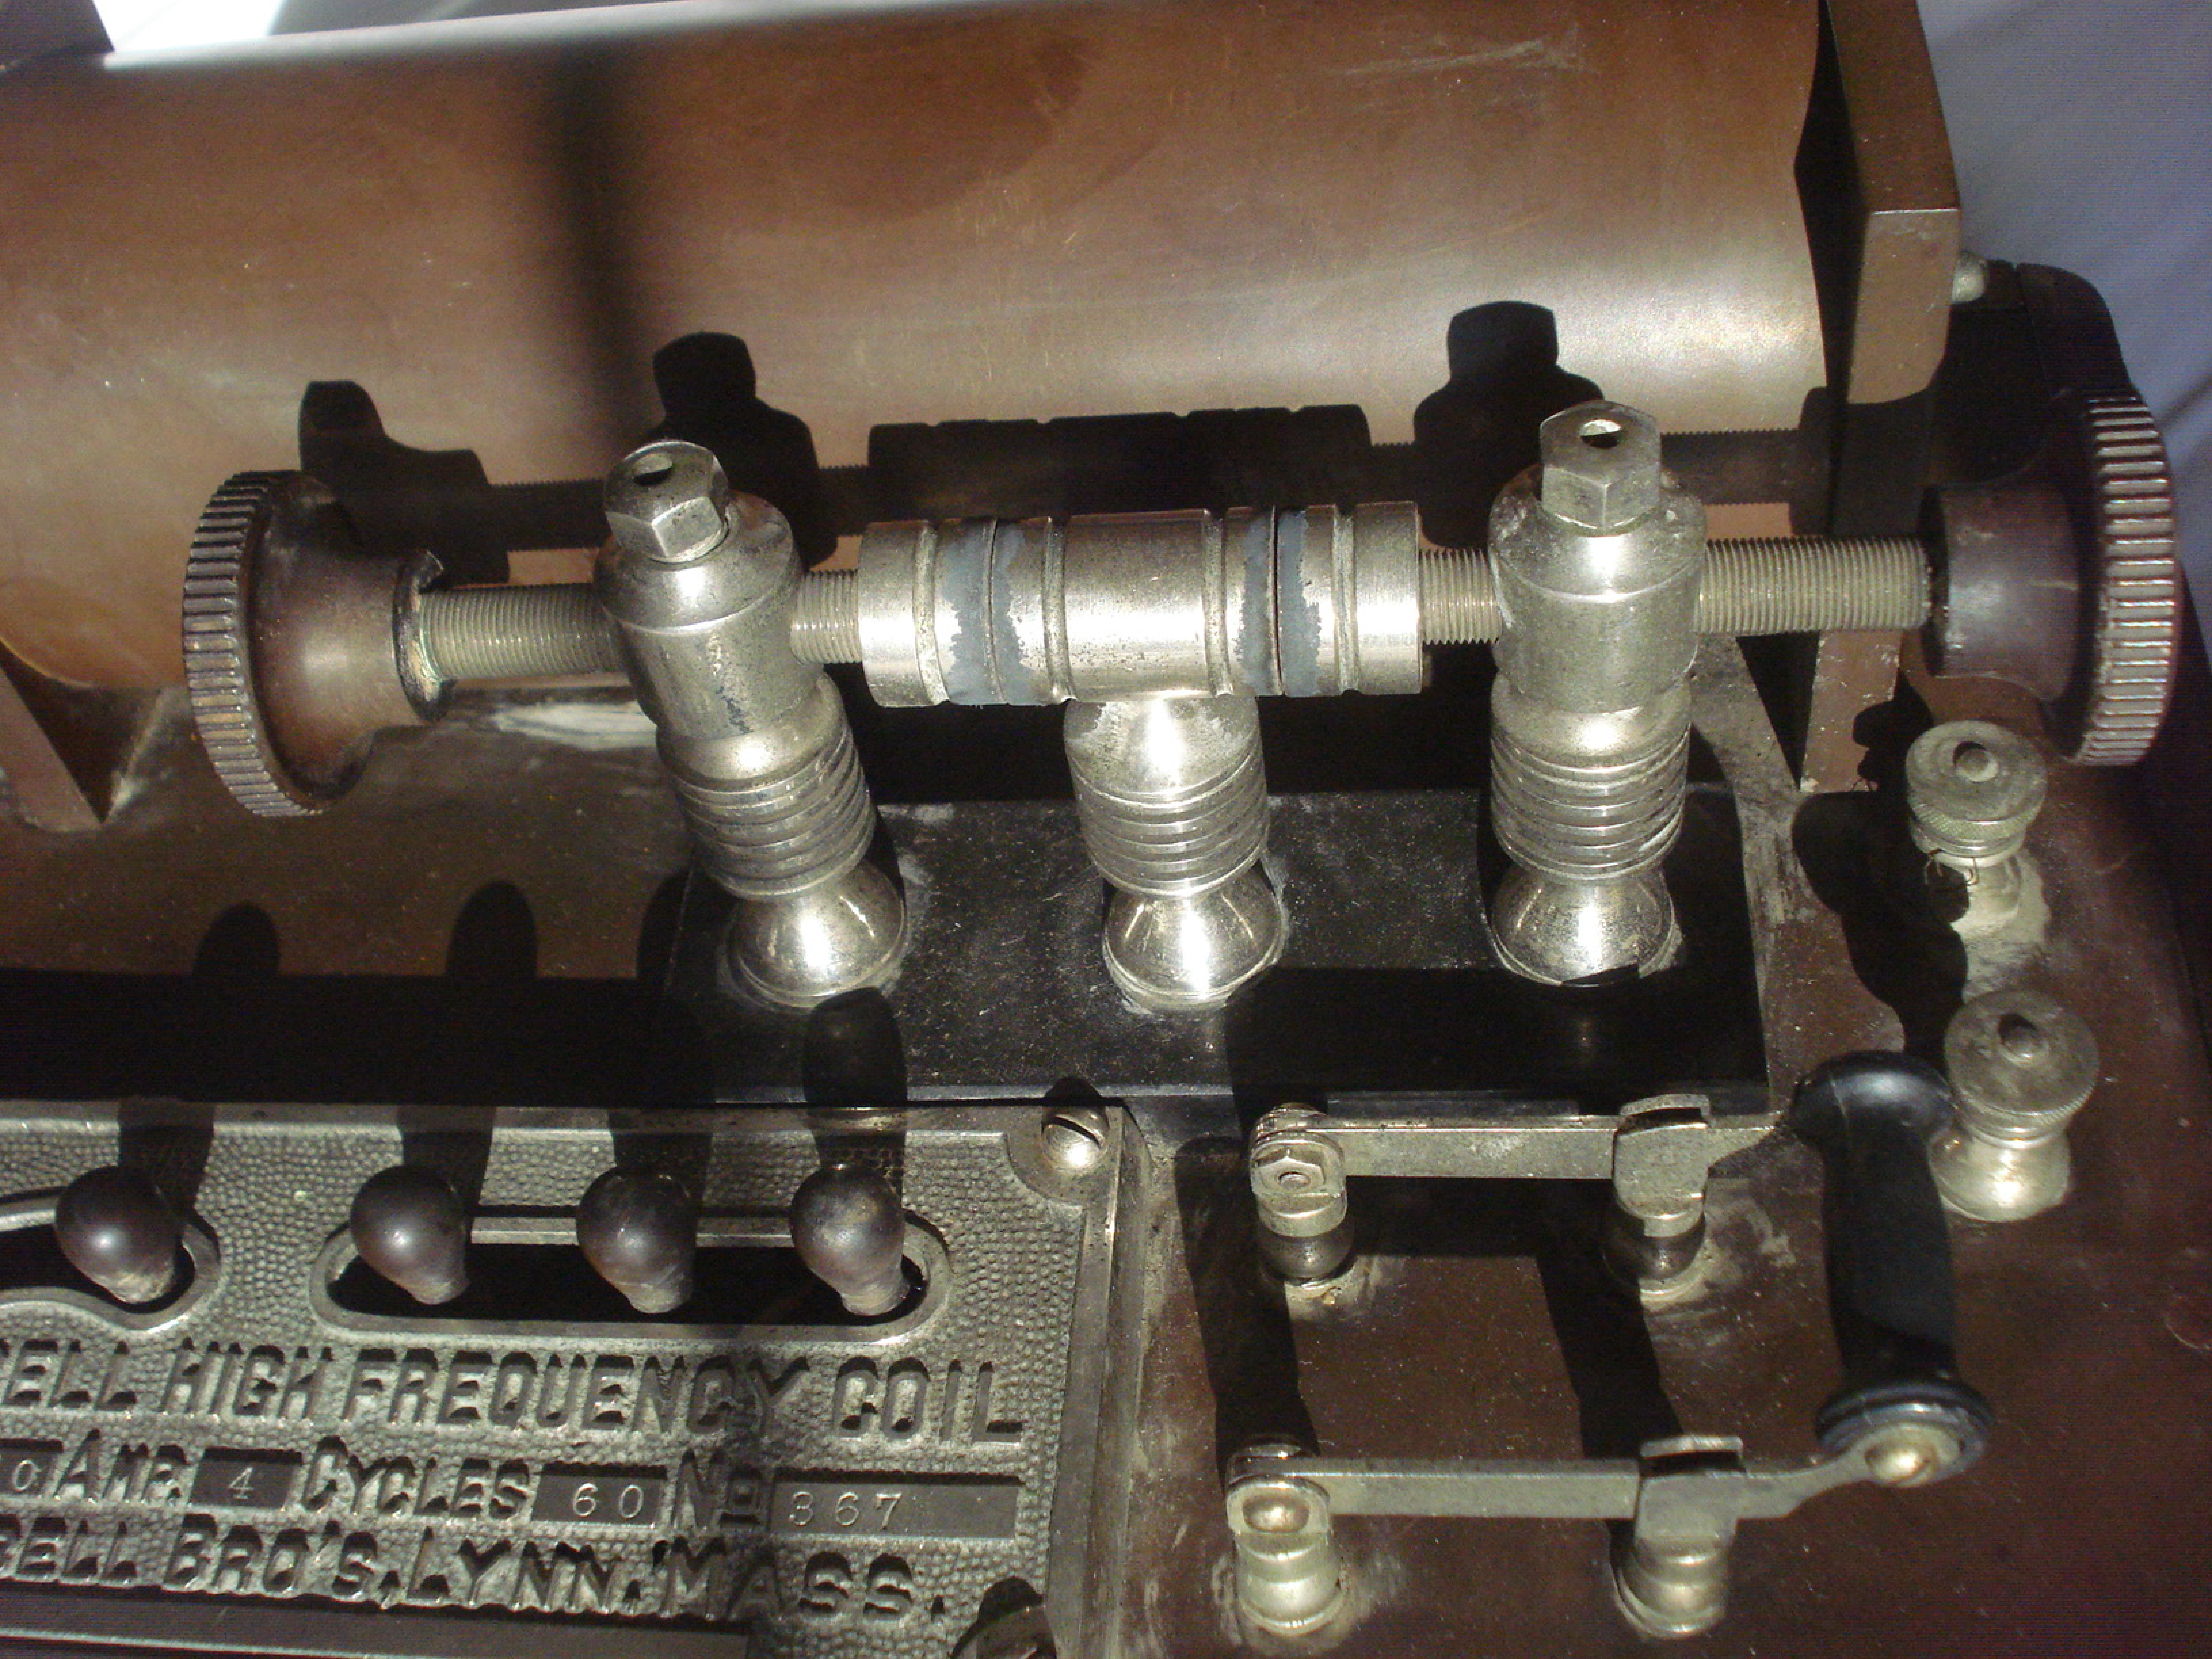
ELL HIGH FREQUENCY COIL
AMP. 4 CYCLES 60 No 367
ELL BRO'S, LYNN, MASS.


CAMPBELL HIGH FREQUENCY COIL
VOLTS 110 AMP. 4 CYCLES 60 No.
CAMPBELL BRO'S. LYNN, MASS.
638

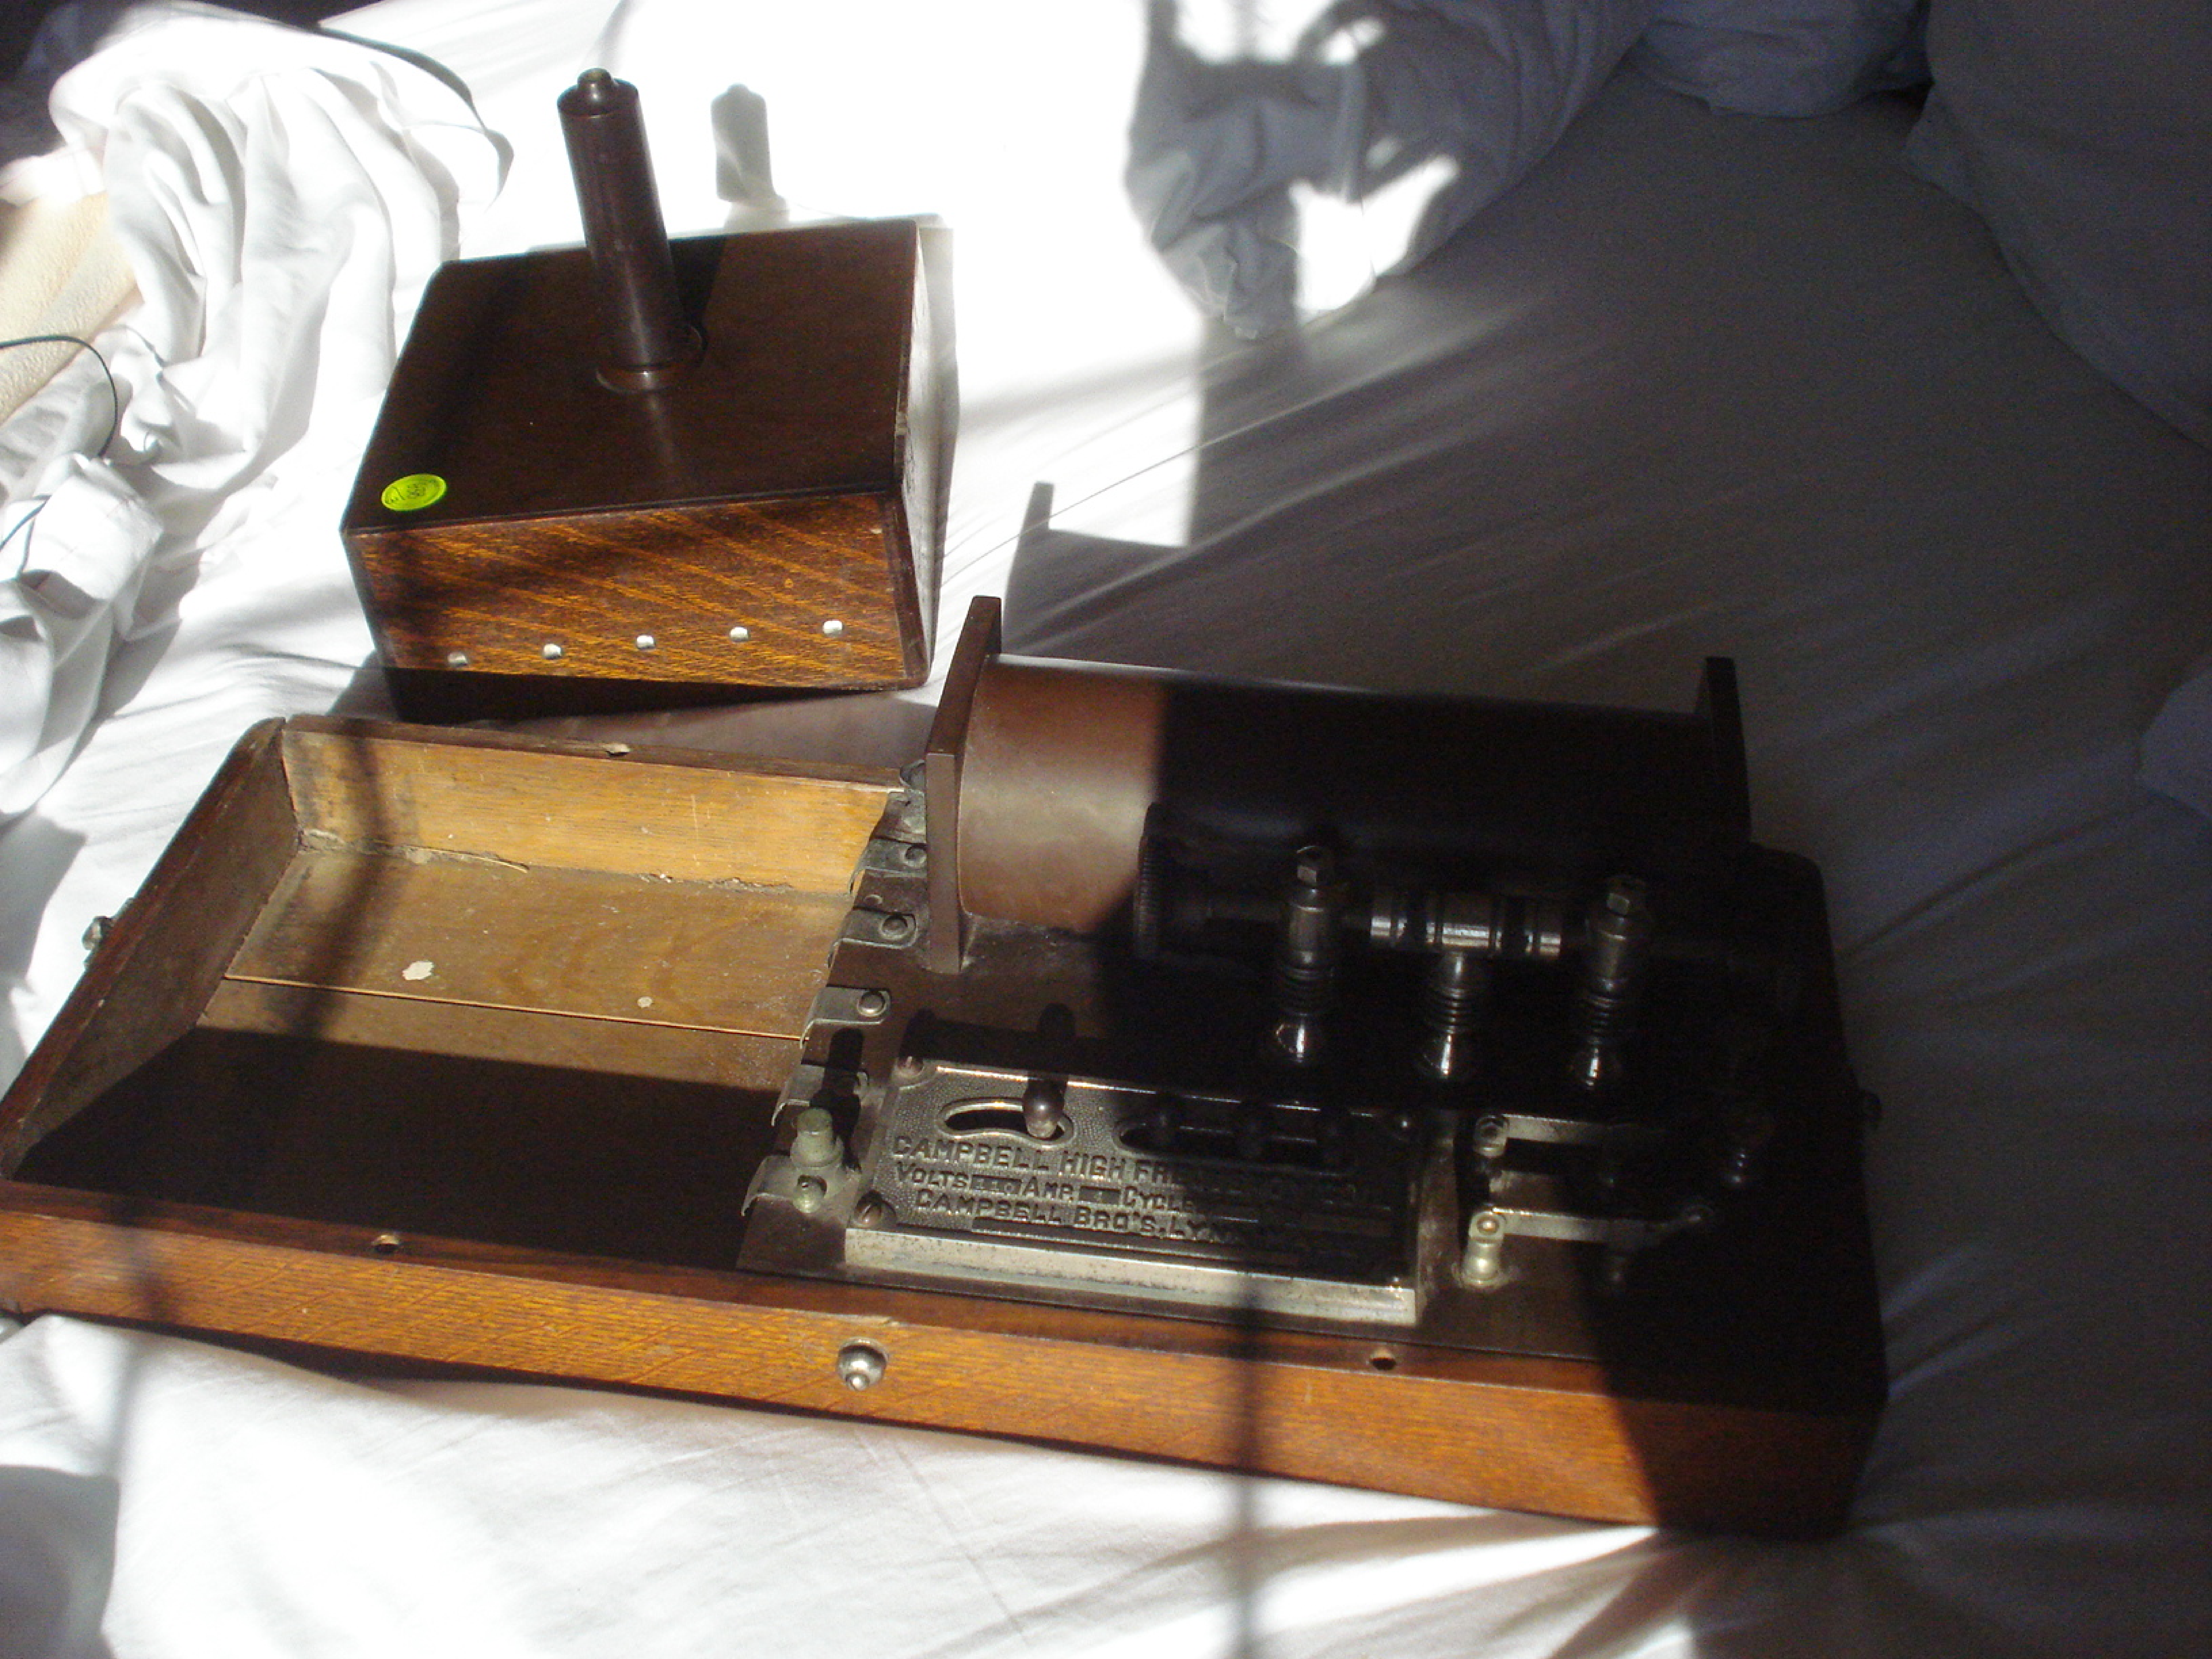
CAMPBELL HIGH
VOLTS AMP.
CAMPBELL BRO'S,

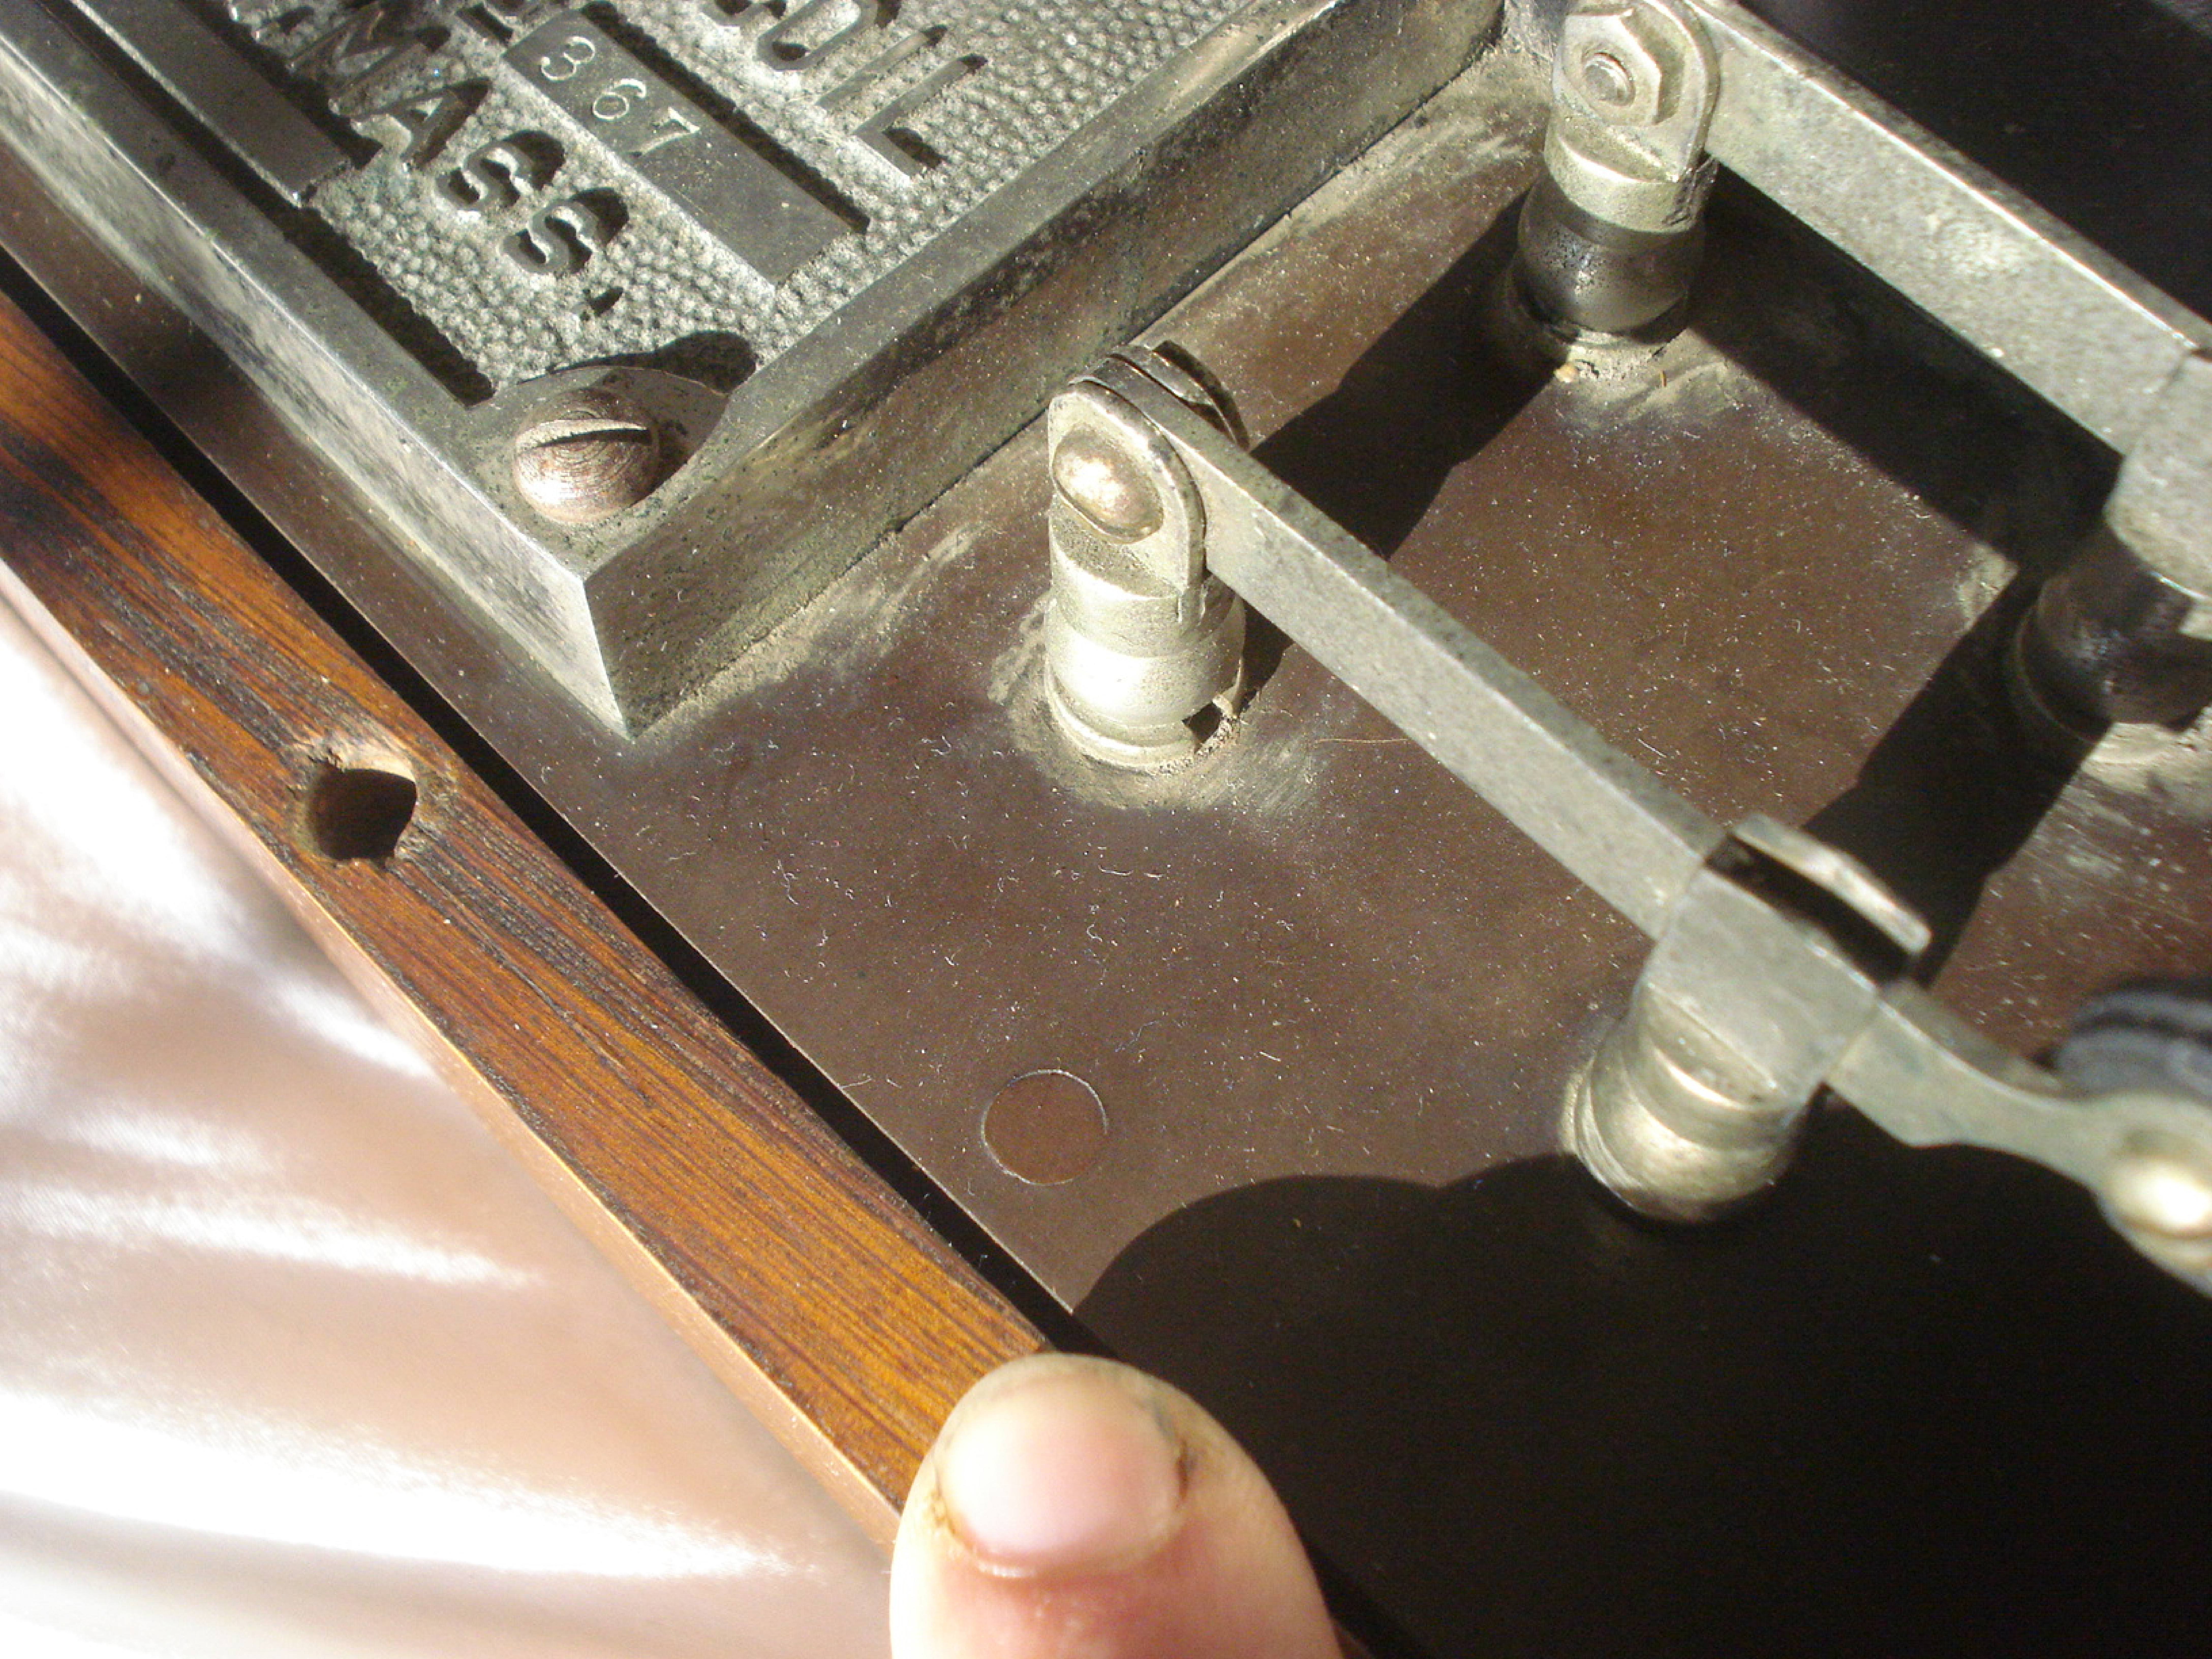


367
MASS


FOR UNIVERSAL OPERATION
CLASS 9TS TUBES
VERTICAL
86° MAX.
NEG. BULB
HORIZONTAL
NEG BRASS BASE
GENERAL ELECTRIC
VAPOR LAMP COMPANY
SEE REVERSE SIDE










FOR UNIVERSAL OPERATION

CLASS 9TS TUBES

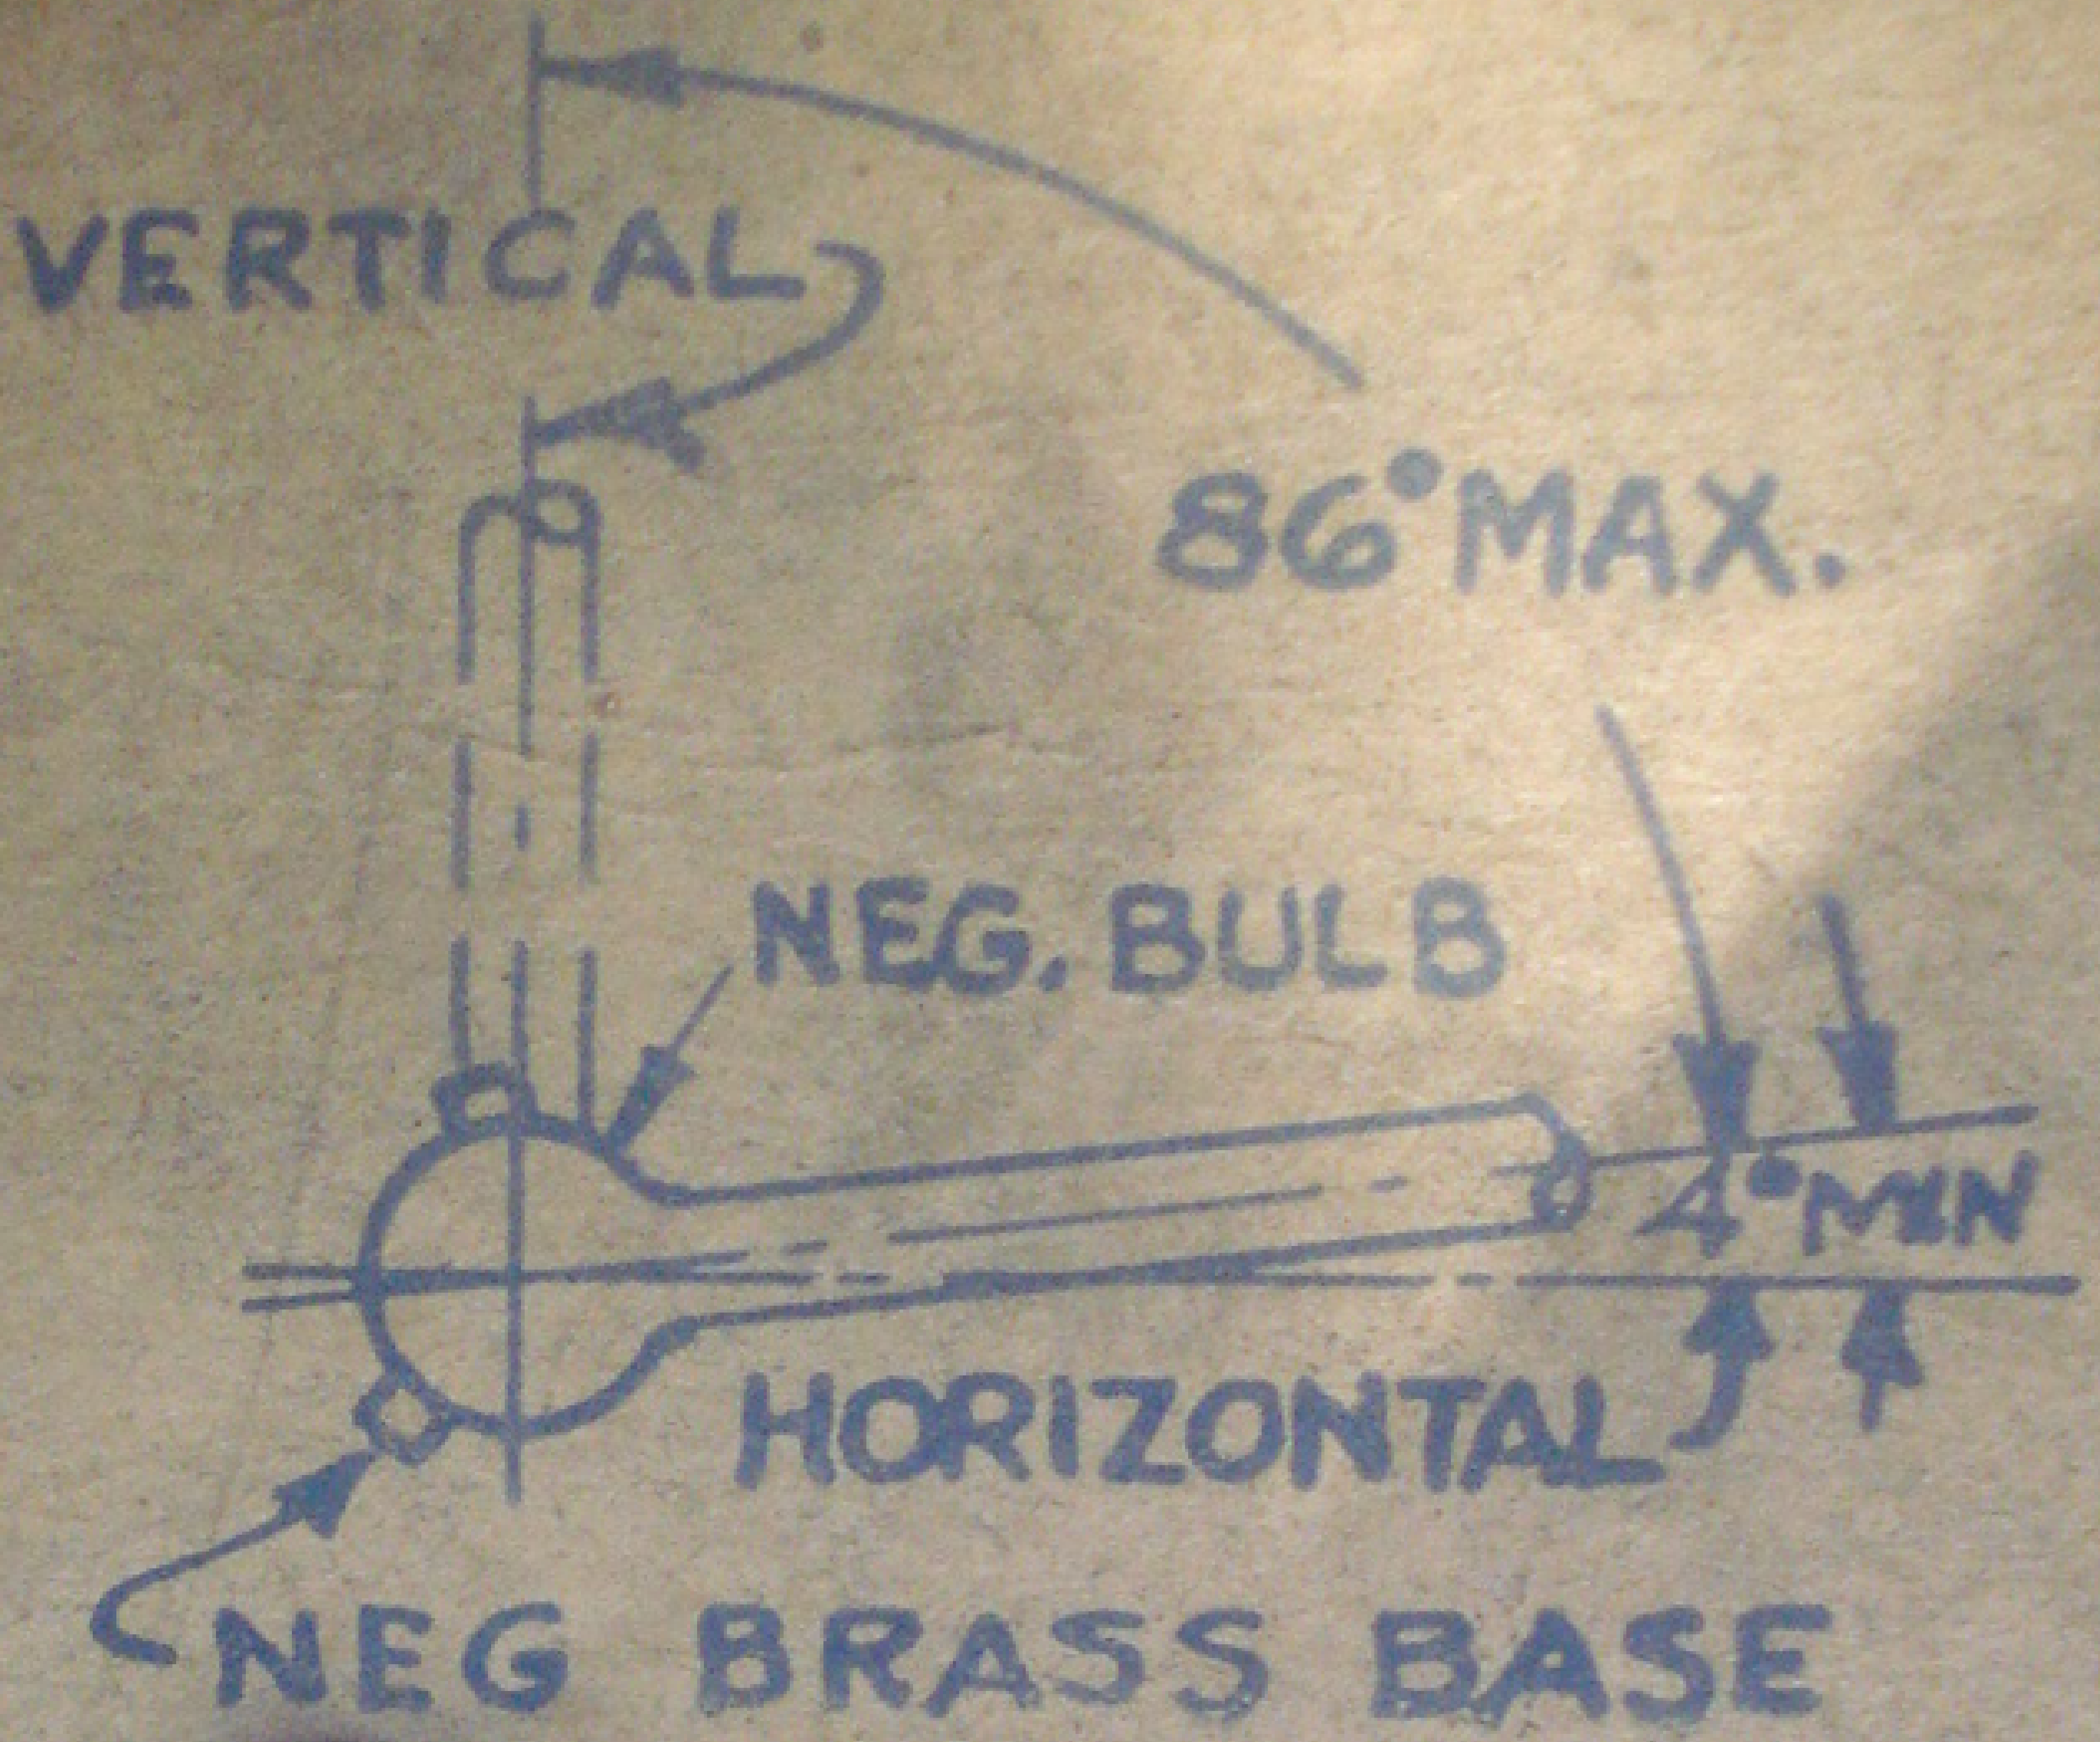

CAUTION:

DO NOT OPERATE BEHIND VERTICAL OR BELOW HORIZONTAL.

GENERAL ELECTRIC VAPOR LAMP COMPANY

HOBOKEN, N. J., U. S. A.

SEE REVERSE SIDE

IMPORTANT

BEFORE INSTALLING TUBE.


1 - REMOVE RUBBER TAPE FROM BOTH ENDS.

2 - WIPE OFF WITH CLEAN DAMP CLOTH.

3 - BE SURE ALL MERCURY IS IN NEGATIVE END.

SEE REVERSE SIDE



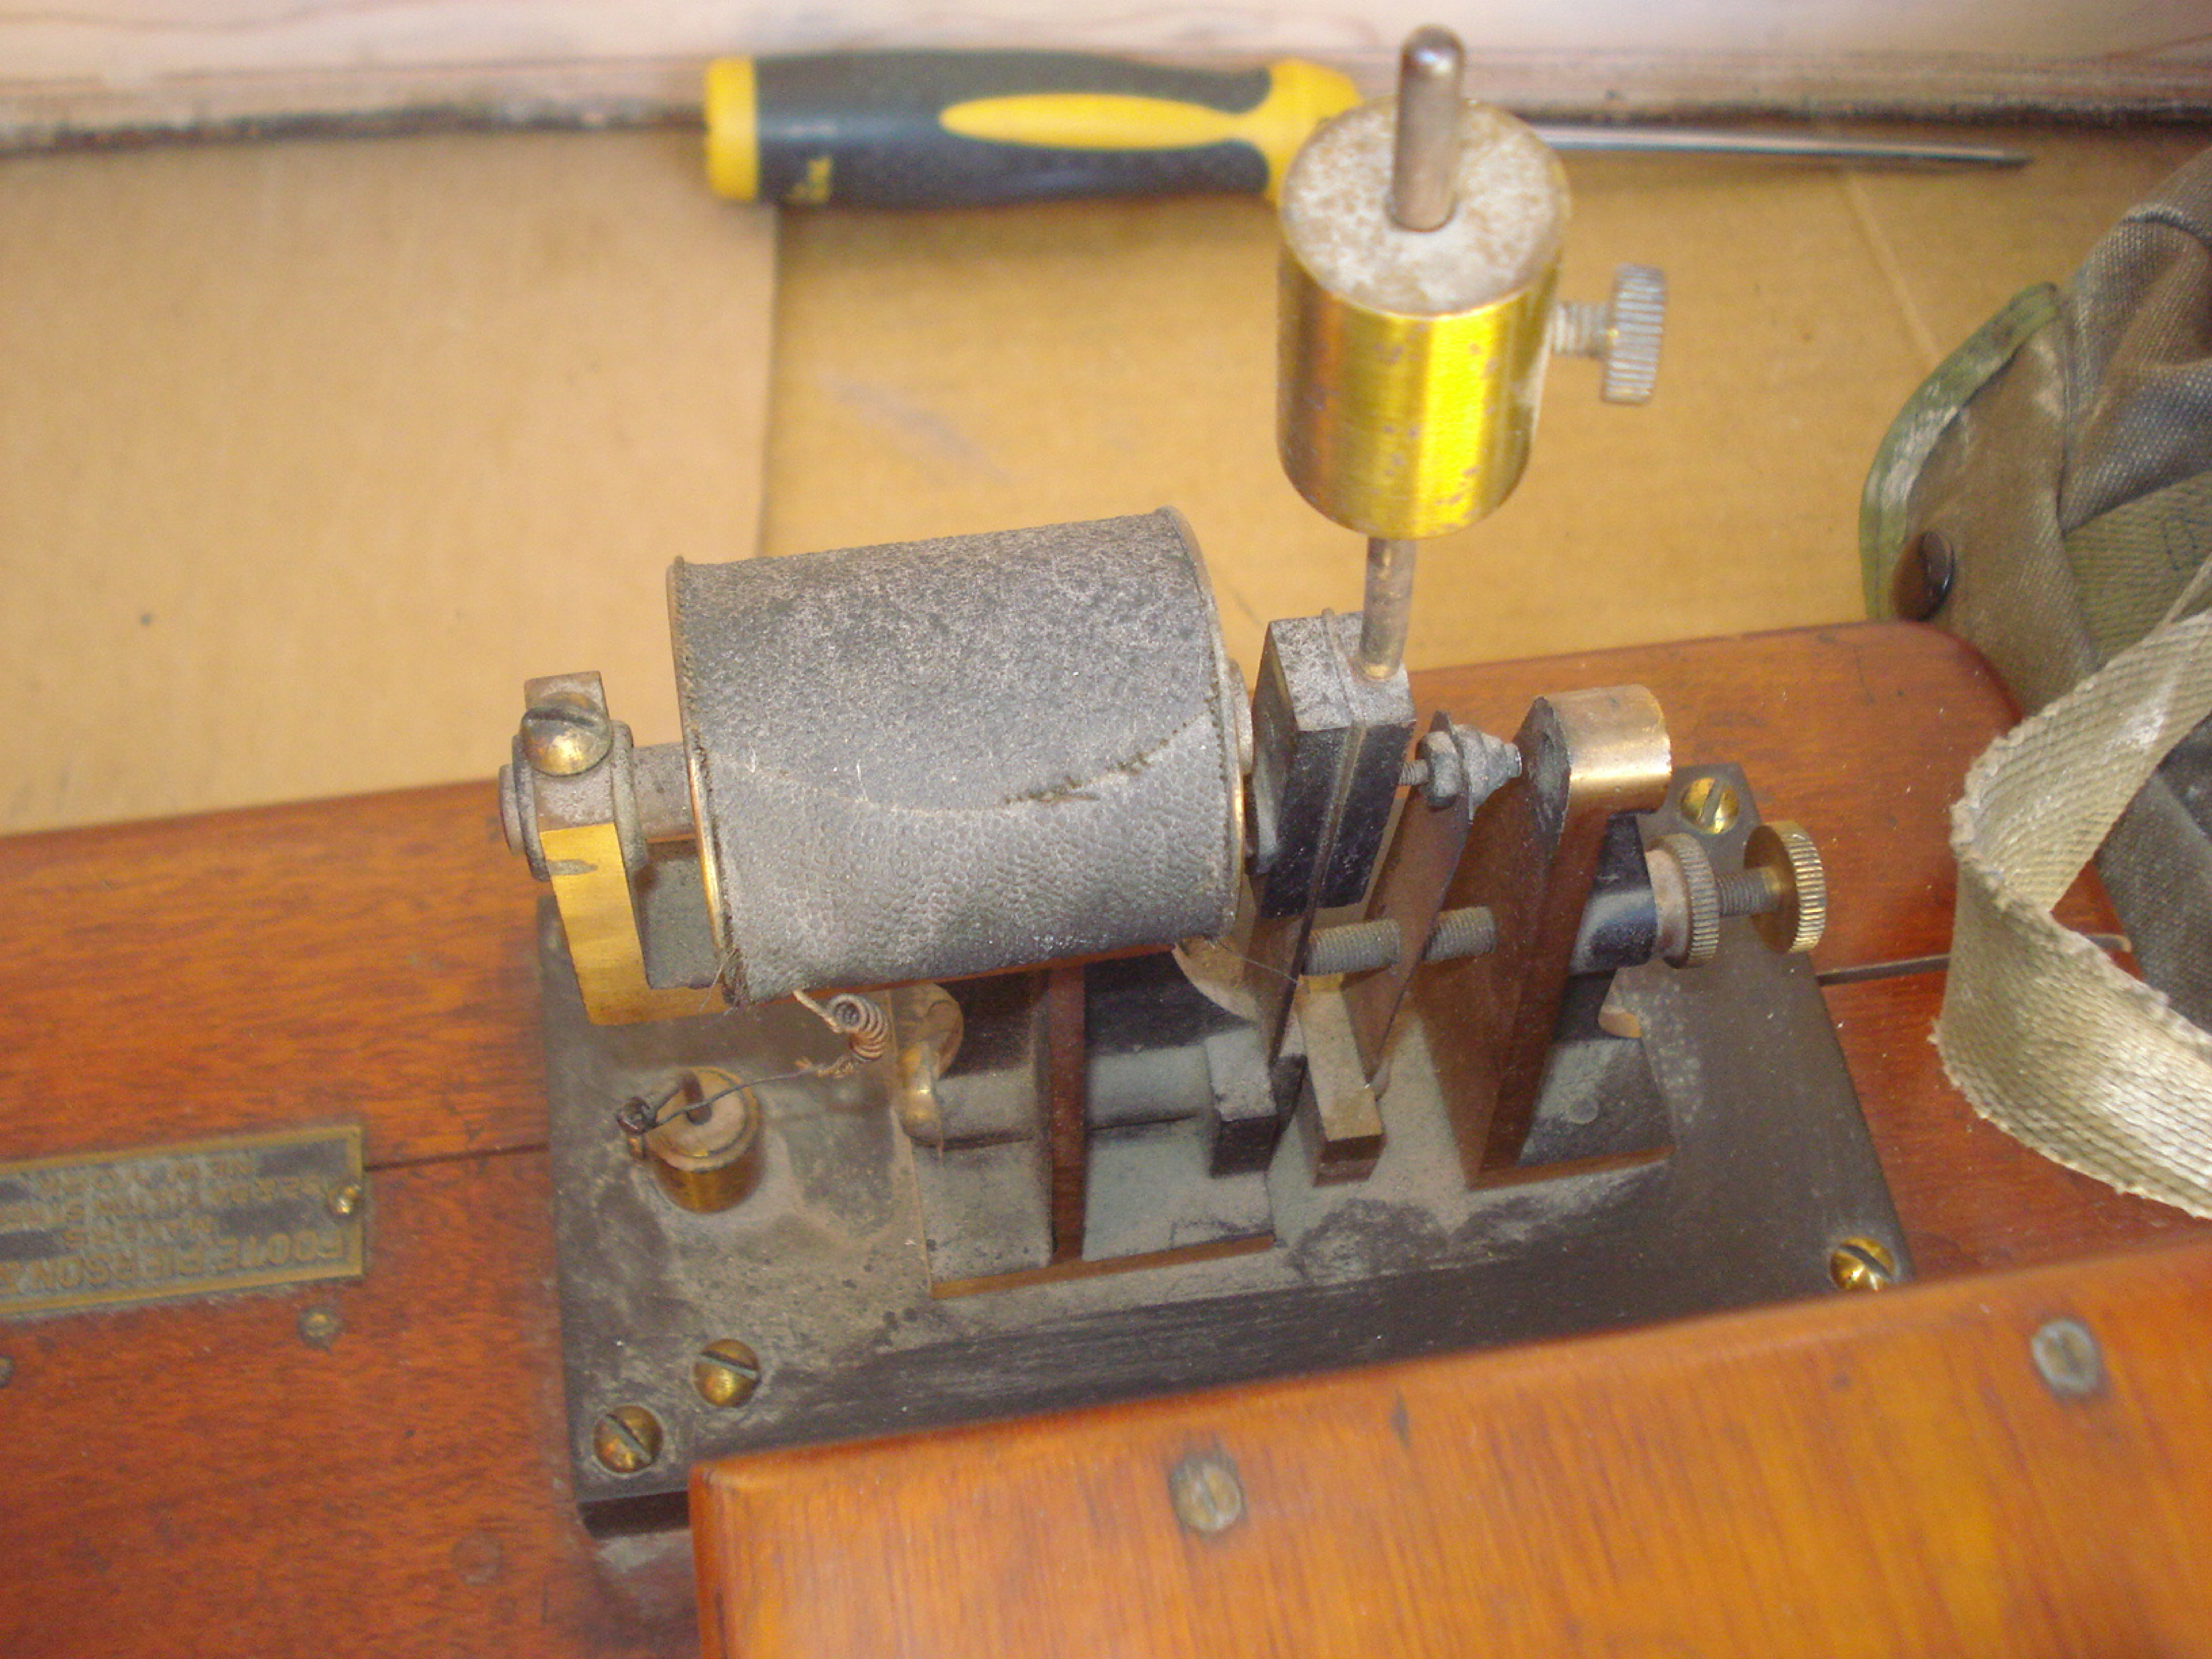






Heavy Duty


OTTO FLEMMING
FARADIC BATTERY
No 4
PHILADELPHIA PA.

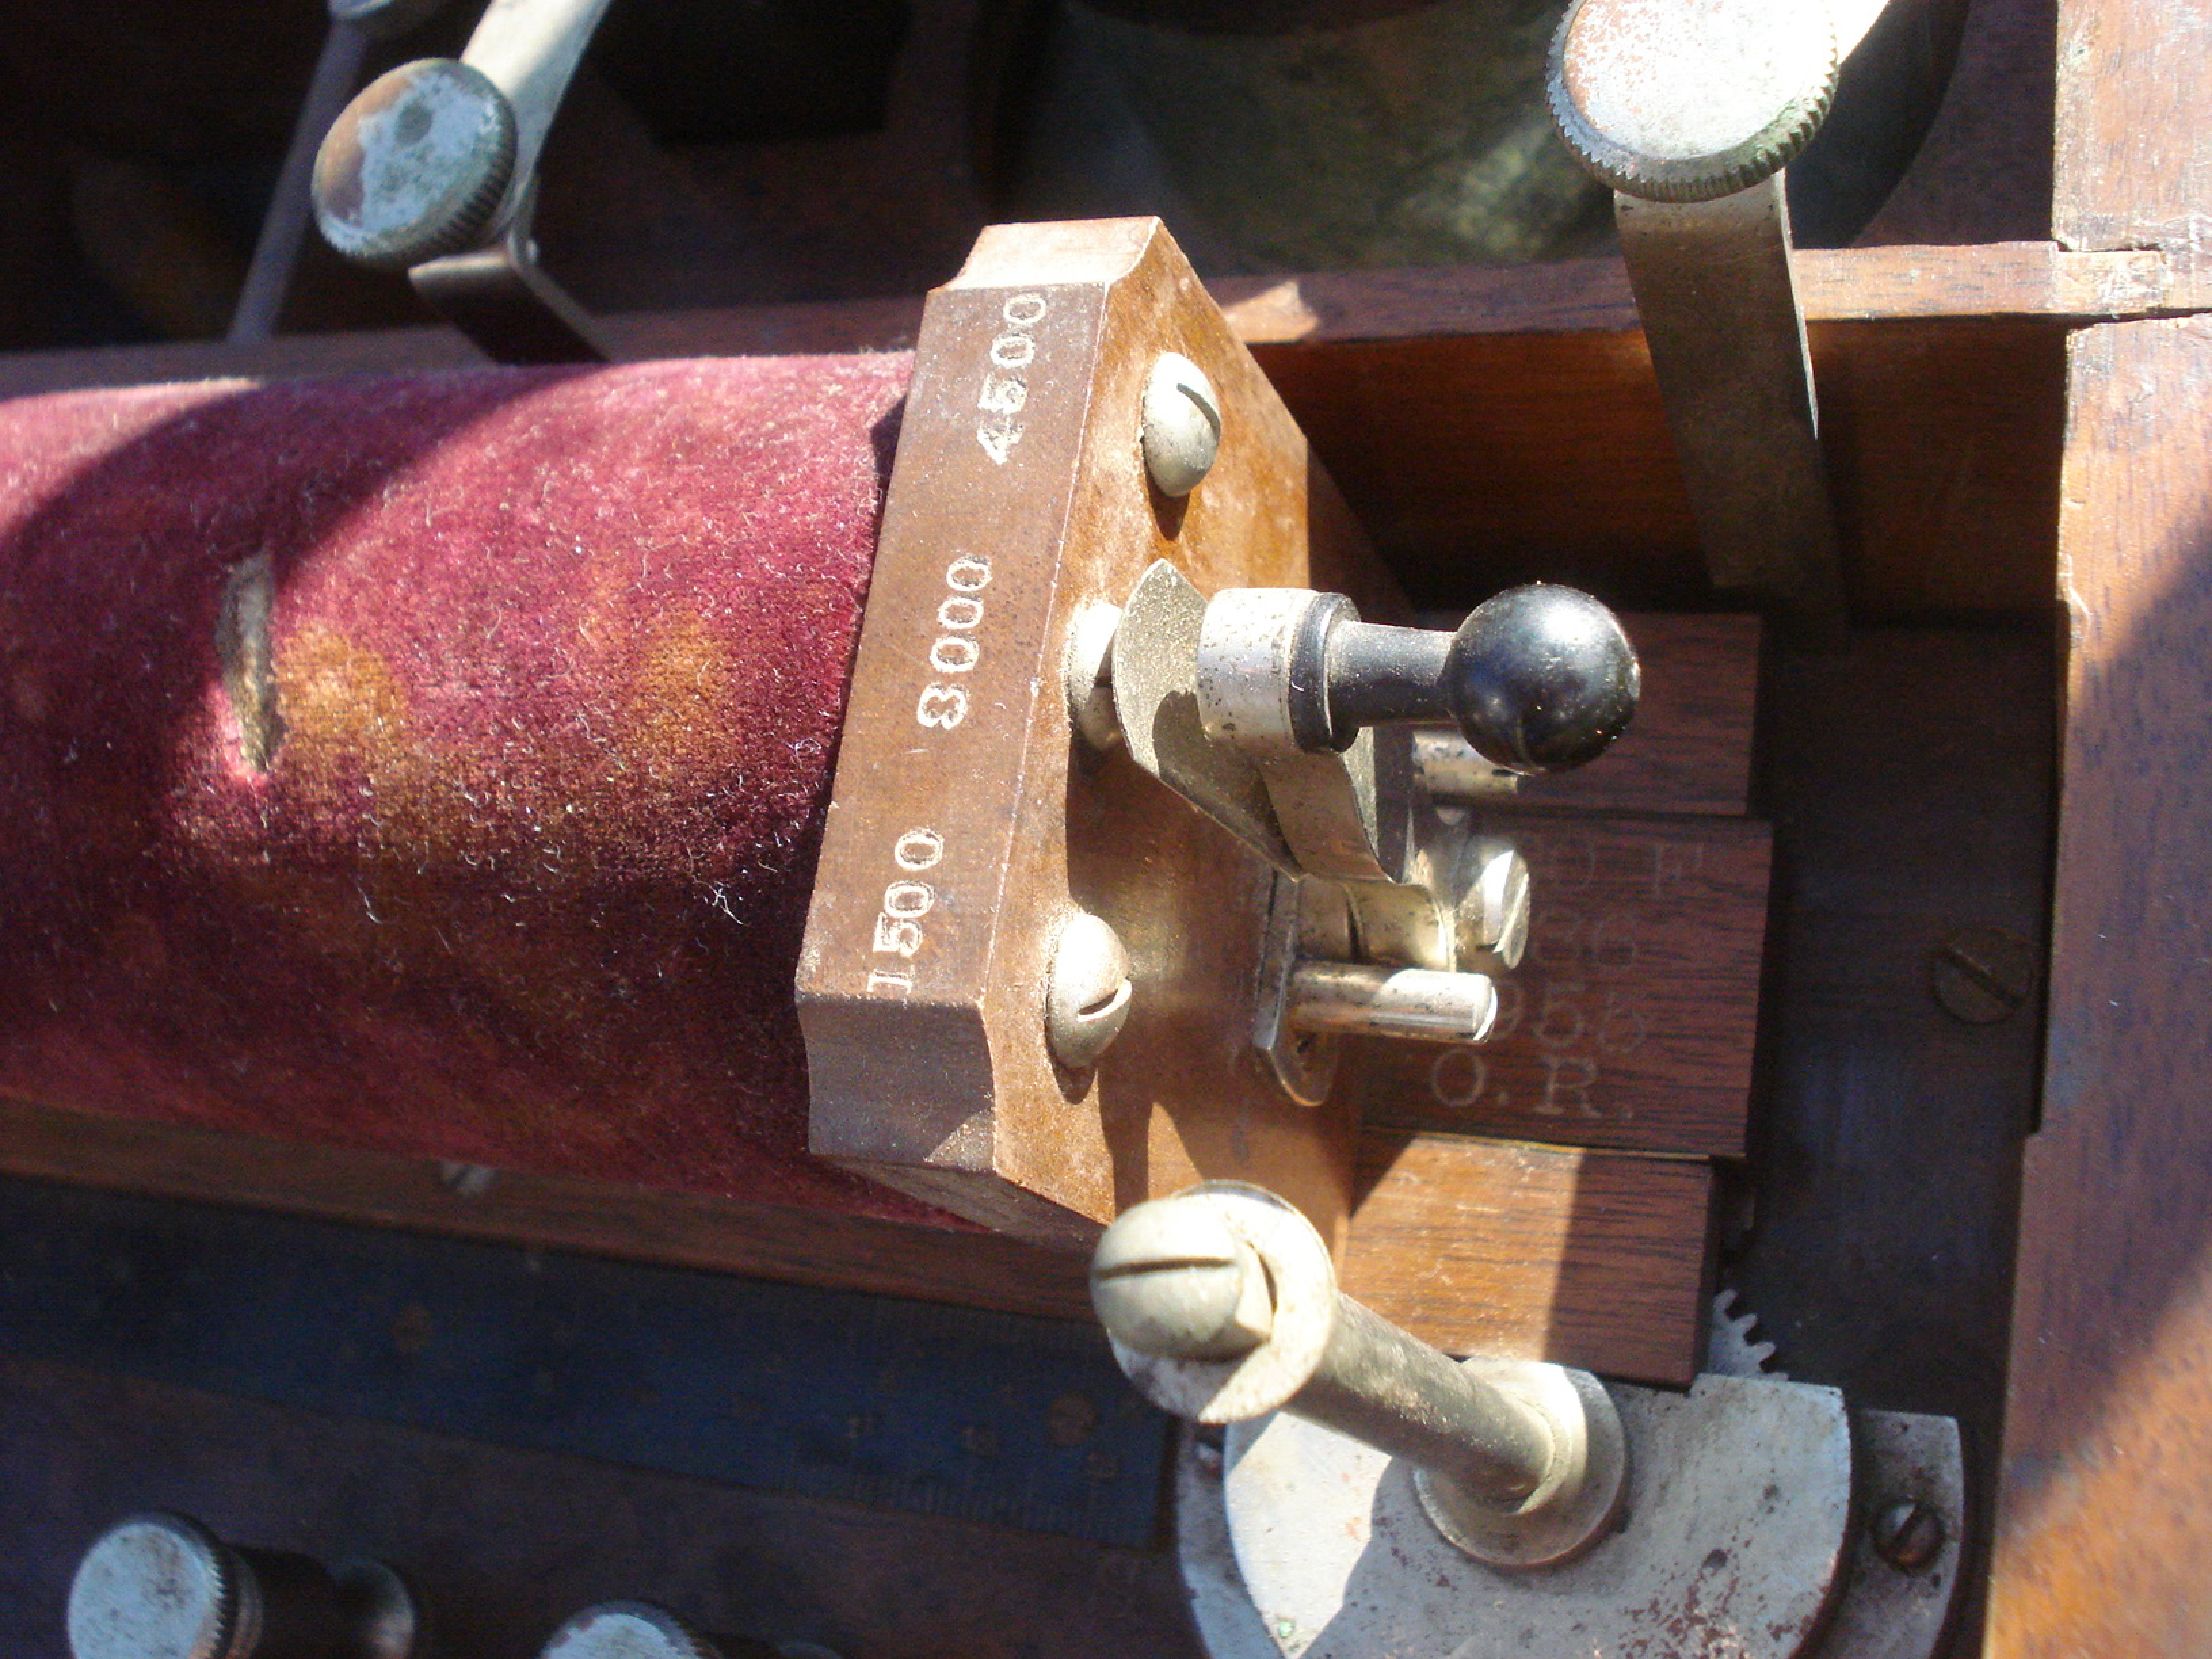


1500
3000
4500

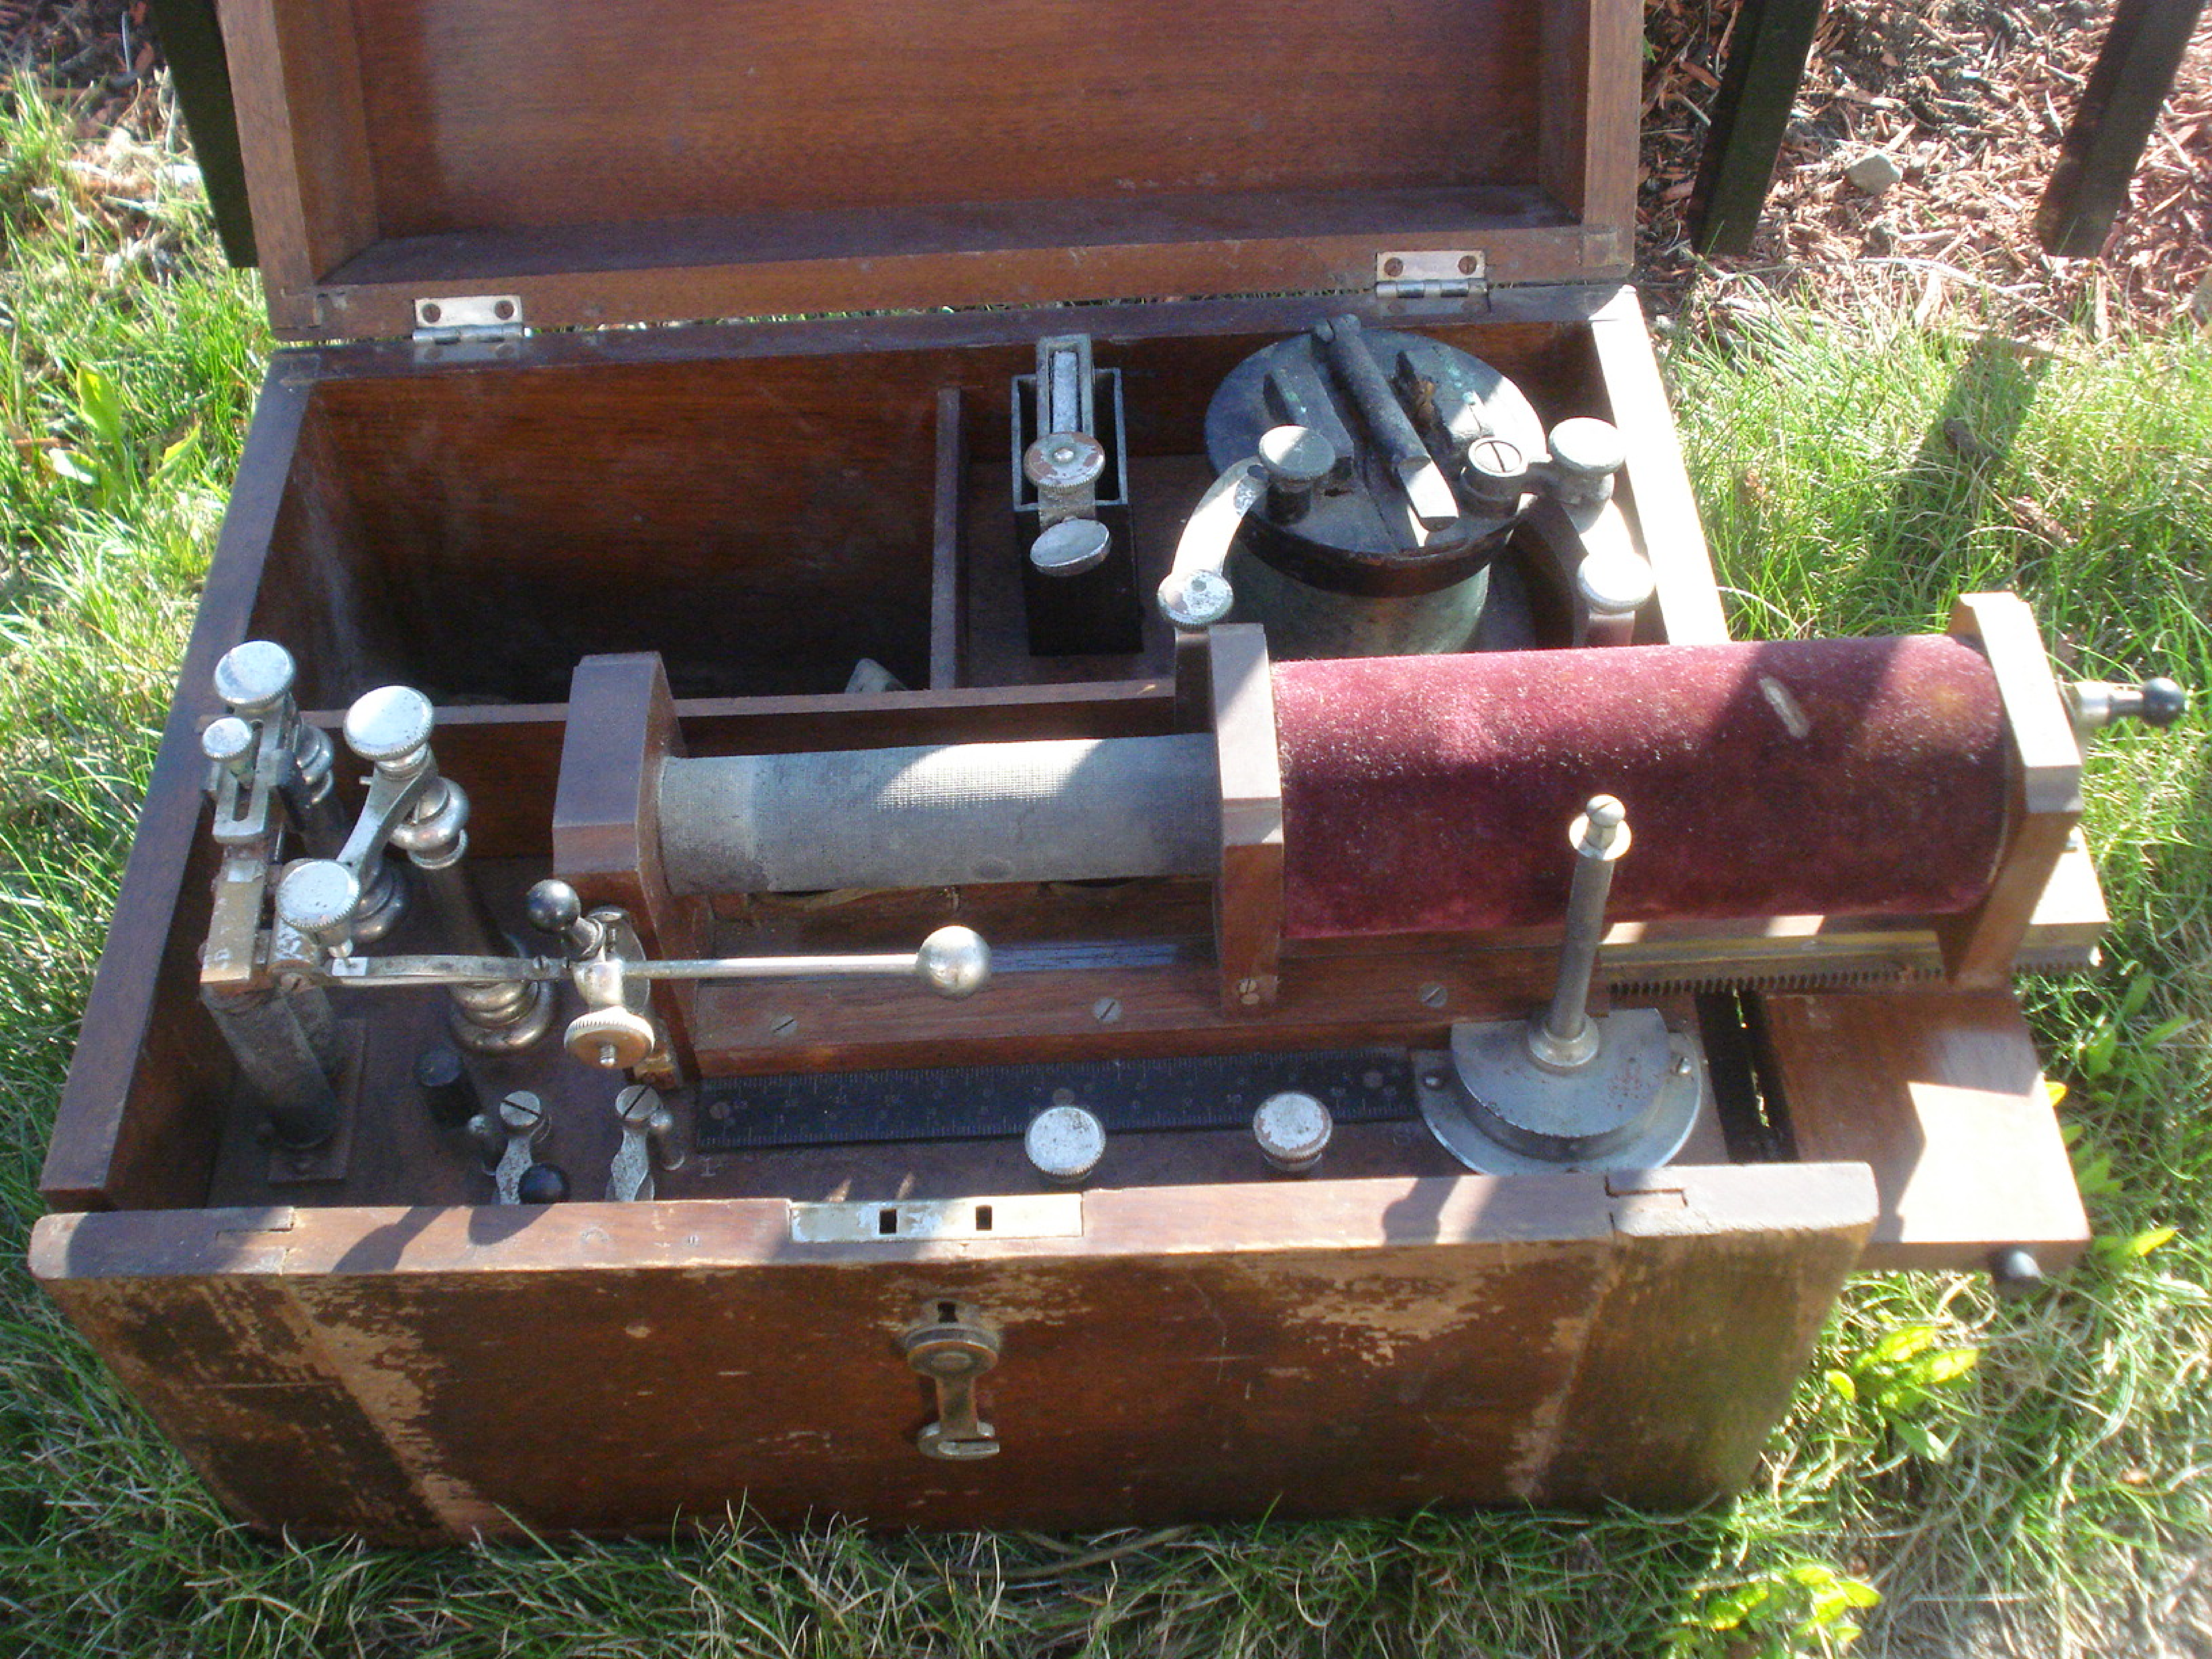


4500
3000






J. KIDDER M'F'G. CO
NEW YORK
ON. OFF
3 2 1


ON
OFF


ON.
OFF.
P
N
J.KIDDER M'F'G.CO.
NEW YORK


CAUTERY
110 V.


CAUTERY
110 V.


LEACH & GREENE
SURGICAL INSTRUMENTS
No. 1 HAMILTON PL.
BOSTON.
Galvano-Faradic-Manufacturing Co.
1131


PRIMARY

Galvano-Faradic M... DR. MOTT.

with yo... Portable Electro Mag-

BY SPECIAL APPOINTM... any cases with entire

Electrical Instrument Mak... MOST COMPLETE AND

TO THE ...vue Hospital ...S. MOTT, M.D.,

Medical College."

NEW YORK STA... ...ESSOR L. BAUER,

FOR NERVOUS ...lege of *Physicians and Surgeons.*

...l me and my professional friends

...*ess, compactness and efficacy*

LOUIS BAUER."

PORTA...

...GARRATT, M. D.,

...e Massac...setts Medical Society.

...gnet... Instrument is truly an excellent

...wagging motion of your vibrator.

...it is the best decidedly of any and

...have seen, giving most distinct

...yet with time enough between to

...twitchings. I shall speak of it

...h shall offer.

ALFRED C. GARRATT."

...the Manufac...

...*very best fo*...

G...

...all respect...

...e, and eas...

Pa...

...PINION ...ay 30, ... CABELL, M. D.,

...of Physiolog... and Surgery, University of Virgini...

...pleasure to bear testimony to the efficiency of...

...Portable Electro-Magnetic Machine. In my e...

...et the expectations raised by the stron...

...of the distinguished medical gentl...

...shed in your pamphlet. Among its...

...being of special inter...

...ets: Compactness...

...battery charge; ...

...current; the very s...

...the current i... at any ...

...rapidity of the interrupti...

...in preventing the least sp...

...perfect cleanliness of the...

...cannot, I think, be surpassed."

Galva...

Galvani...

...he *LECTR*...

...com...

...the...

...dimini...

...tens... EAST ...

...n...


BOSTON.
Galvano-Faradic Manufacturing Co.
East 34th-Street
NEW-YORK.

ND.

lege, Philadelphia.

st at the Philadelphia
anic and Faradic In-

RAINS.

e of Augusta, Georgia
Magnetic Machine and in-
n August last, and design
the class of Medical Stu-
peutics during the present

MURRAY.

Magnetic Machine for some
twelve months in my office
any other electrical instru-

BLUM ENTHAL.

ad in daily use, the various

"I used the
Hospital, with
struments also gi

SPECIAL ANNOUNCEMENT.

Additional Letters-Patent, Issued March 26, 1872.

THE PORTABLE
ELECTRO-MAGNETIC MACHINE.

REDUCED IN SIZE ONE-THIRD—IN WEIGHT NEARLY ONE-HALF.
INCREASED IN VOLUME, POWER, AND EFFICACY.
THE CURRENTS FLOW WITH UNEQUALLED SMOOTHNESS, EVENNESS, AND DELICACY, AND CAN BE INSTANTLY AND UNERRINGLY CHANGED FROM PRIMARY TO SECONDARY—FROM POSITIVE TO NEGATIVE.

WE take great pleasure in announcing the Completion of our Portable Electro-Magnetic Machine. Every effort ha... irrespective of Expense or Ex...



JEROME KIDDER
INVENTOR
PAT IN ENGLAND
PAT IN FRANCE
NEW YORK
793
4
AUCTIONEERS


DR. JEROME KIDDER
INVENTOR
March 15 1864
Jan 16 1866 Sept 18 1866
Aug. 10 1869
Jan 4 1876
PAT. IN ENGLAND
July 31
1865
PAT. IN FRANCE
Aug. 3
1865
NEW YORK




A
B
PAT. FEB
1876





SWETT & LEWIS


THE KINRAIDE COIL
MANF'D BY
HOWARD Jr JACKSON CO.
SWETT & LEWIS
BOSTON, MASS. U.S.A.
CYCLES
PATENTED


VOLTS 110
NO.17065 D
SPEED


OIL


THE KINRAIDE COIL
MANF'D BY
HOWARD JACKSON
FOR
SWETT & LEWIS CO.
BOSTON, MASS., U.S.A.
NO. 135 V. 110 CYCLES
PATENTED








OIL







OIL
KINRAIDE CO
WETT & LEWIS
BOSTON, MASS.
CYCLES
PATENTED




KINRAIDE


THE KINRAIDE


VOLTS 110
NO.17065D
SPEED




















THE
HOWARD


THE KINRAID
HOWARD JAC




THE KINRAI
MANF'D
HOWARD J
FOR
SWETT & LE
BOSTON, MAS
NO.
V.
PATENT
OIL


VOLTS 110
NO.17065D
SPEED
L#1








TO BROTHER
Thomas
THIS CUP IS GIVEN BY THE
MEMBERS OF THE WILLIAMS CLUB
IN APPRECIATION OF MANY COURTESIES
SHOWN THEM WHILE HIS GUESTS AT
"The Hermitage"
SANDWICH MASS.
JUNE 12-13, 1909
MAY YOU LIVE LONG AND PROSPER


THIS CUP IS GIVEN BY THE
MEMBERS OF THE WILLIAMS CLUB
APPRECIATION OF MANY COURTESIES
"The Hermitage"
MASS
YOU LIVE LONG AND PROSPER


ASHMAN
BARLOW
KINGSBURY
PAUL·C
LEMUEL
JOHN·S
LIONEL·E


ALFRED · A · ASHMAN
MYRON · BARLOW
GEORGE · W · HETHERINGTON
CHARLES · H · KINGSBURY
ANTON · F · KOERNER
HERMAN · F · KLEIN
PAUL · C · KLEIN
LEMUEL · H
JOHN · S
LIONEL · E
GEORGE


FREDERIC H PERRY
WILLIAM F PINKHAM
CHARLES W TABER
EUGENE C UPTON
IRVING E WILLIAMS
ARTHUR H WOODCOCK
WILLIAM K DAVIDSON






TeamViewer 8
Skype
ZD55X1000...
CalTool
ScanPattern
zinFrame Panel
ZD55X1000214DFA
General
Advanced
Fine Tuning
About
Calibration
Diagnose
Servicing interface control established.
OK
Cancel
Apply
Programs
Folders
Windows Compatibi...
Angry Birds Rio
Bing Maps 3D
EditPlus 3
Runespell Overture
Fruit Ninja
World of Goo
Torchlight
BIT.TRIP BEAT
d20Pro-2
Arena
Snowflake
Plants vs. Zombies
Monopoly
Bejeweled 3
Files & Documents
Steam
WinSCP
Google Chrome
Acrobat Reader 5.0
putty
WindowBli...
Dropbox
IdentityMine Sand
Play More Great Games!


TO BROTHER
Thomas Burton Kinraide
THIS CUP IS GIVEN BY THE
MEMBERS OF THE WILLIAMS CLUB
IN APPRECIATION OF MANY COURTESIES
SHOWN THEM WHILE HIS GUESTS AT
"The Hermitage"
MASS
MAY YOU LIVE LONG AND PROSPER


THIS CUP IS
MEMBERS OF THE
APPRECIATION OF
SHOWN THEM WHILE
MASS
YOU LIVE


ALFRED · A · ASHMAN
MYRON · BARLOW
W · HETHERINGTON
CHARLES · H · KINGSBURY
ANTON · F · KOERNER
HERMAN · F · KLEIN
PAUL · C · KLEIN
LEMUEL · H
JOHN · S


FREDERIC·H·PERRY
WILLIAM·F·PINKHAM
C·J·POPE
AUGUST·F·SCHERER
CHARLES·W·TABER
EUGENE·C·UPTON
IRVING·E·WILLIAMS
ROBERT·G·WILSON
ARTHUR·H·WOODCOCK
WILLIAM·K·DAVIDSON


MEMBERS OF THE


ALFRED·A·ASHMAN
BARLOW
W·HETHERINGTON
CHARLES·H·KINGSBURY
ANTON·F·KOERNER
HERMAN·F·KLEIN
PAUL·C·KLEIN
LEMUEL·H
JOHN·S
LIONEL·E
GEORGE·E








BACON
MAKES IT


BACON
MAKES IT

AMERICAN INSTITUTE
of
ELECTRICAL ENGINEERS



WALDORF ASTORIA
New York

January 13, 1902

Alexander Graham Bell Jan. 13 1902
M. I. Pupin
Guglielmo Marconi
Charles P. Steinmetz
Elihu Thomson
Percy Sanderson
F. B. Crocker
T. C. Martin
Marian H. Graham Bell
Gilbert H. Grosvenor
E. W. Parker
Maud M. Hill
J. McKee

ANNUAL DINNER

.. .. of .. ..

THE AMERICAN INSTITUTE OF ELECTRICAL ENGINEERS

GUEST OF HONOR

Signor Guglielmo Marconi

Cav. della Corona d'Italia

Member, Institution of Electrical Engineers, London

Member, Società Italiana delle Scienze detta dei Quaranta, Rome

Member, Associazione Elettrotecnica Italiana, Rome

MENU

Huitres

Potage Electrolytique

Hors d'oeuvres

Radis Olives Céleri Amandes Salées

Filet de Bass à la Chevalière

Tomates farcies aux concombres

Volaille et Champignons frais à la Suzette

Filet de boeuf piqué, Sauce au Madère

Pommes de terre rissolées Haricots verts panachés

Pamplemousse au marasquin

Canard tête noire rôti

Gelée de Groseilles Hominy frit

Salade de Romaine

Glaces de fantaisie Gâteaux assortis


Fruits


Café

Cigares Cigarettes


KEY WEST


THE ELLI
The Vibrophone
808

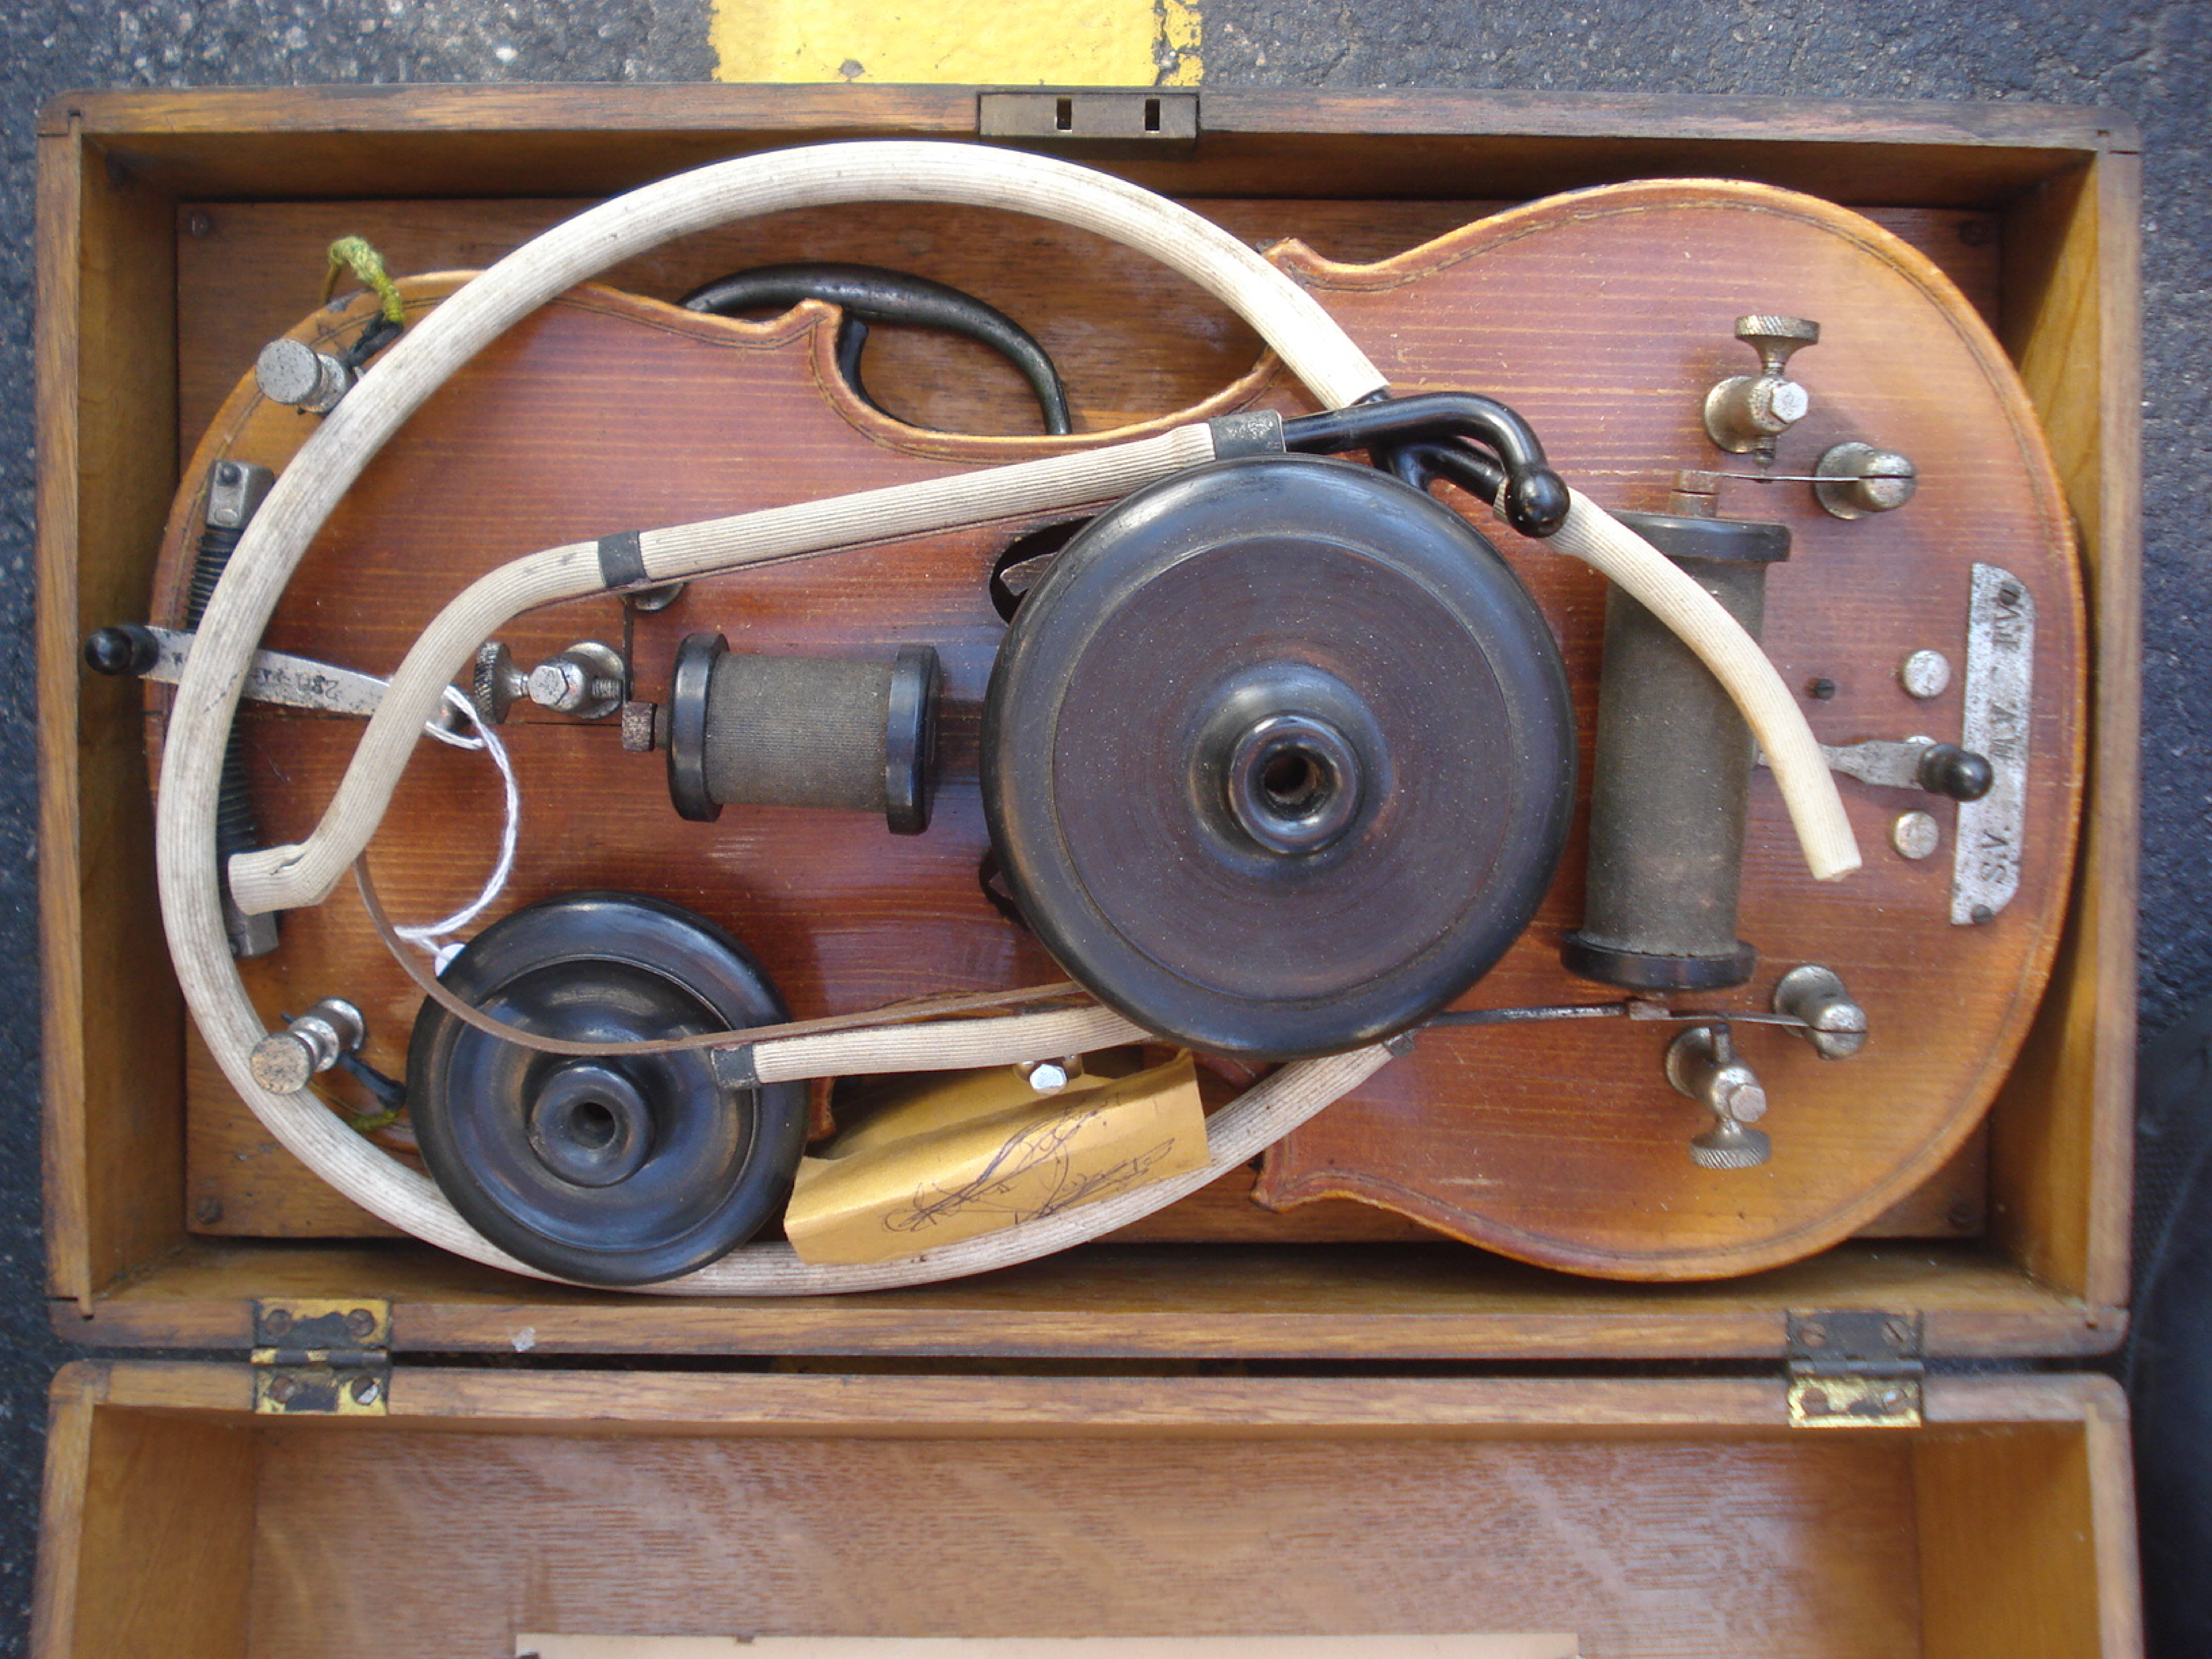

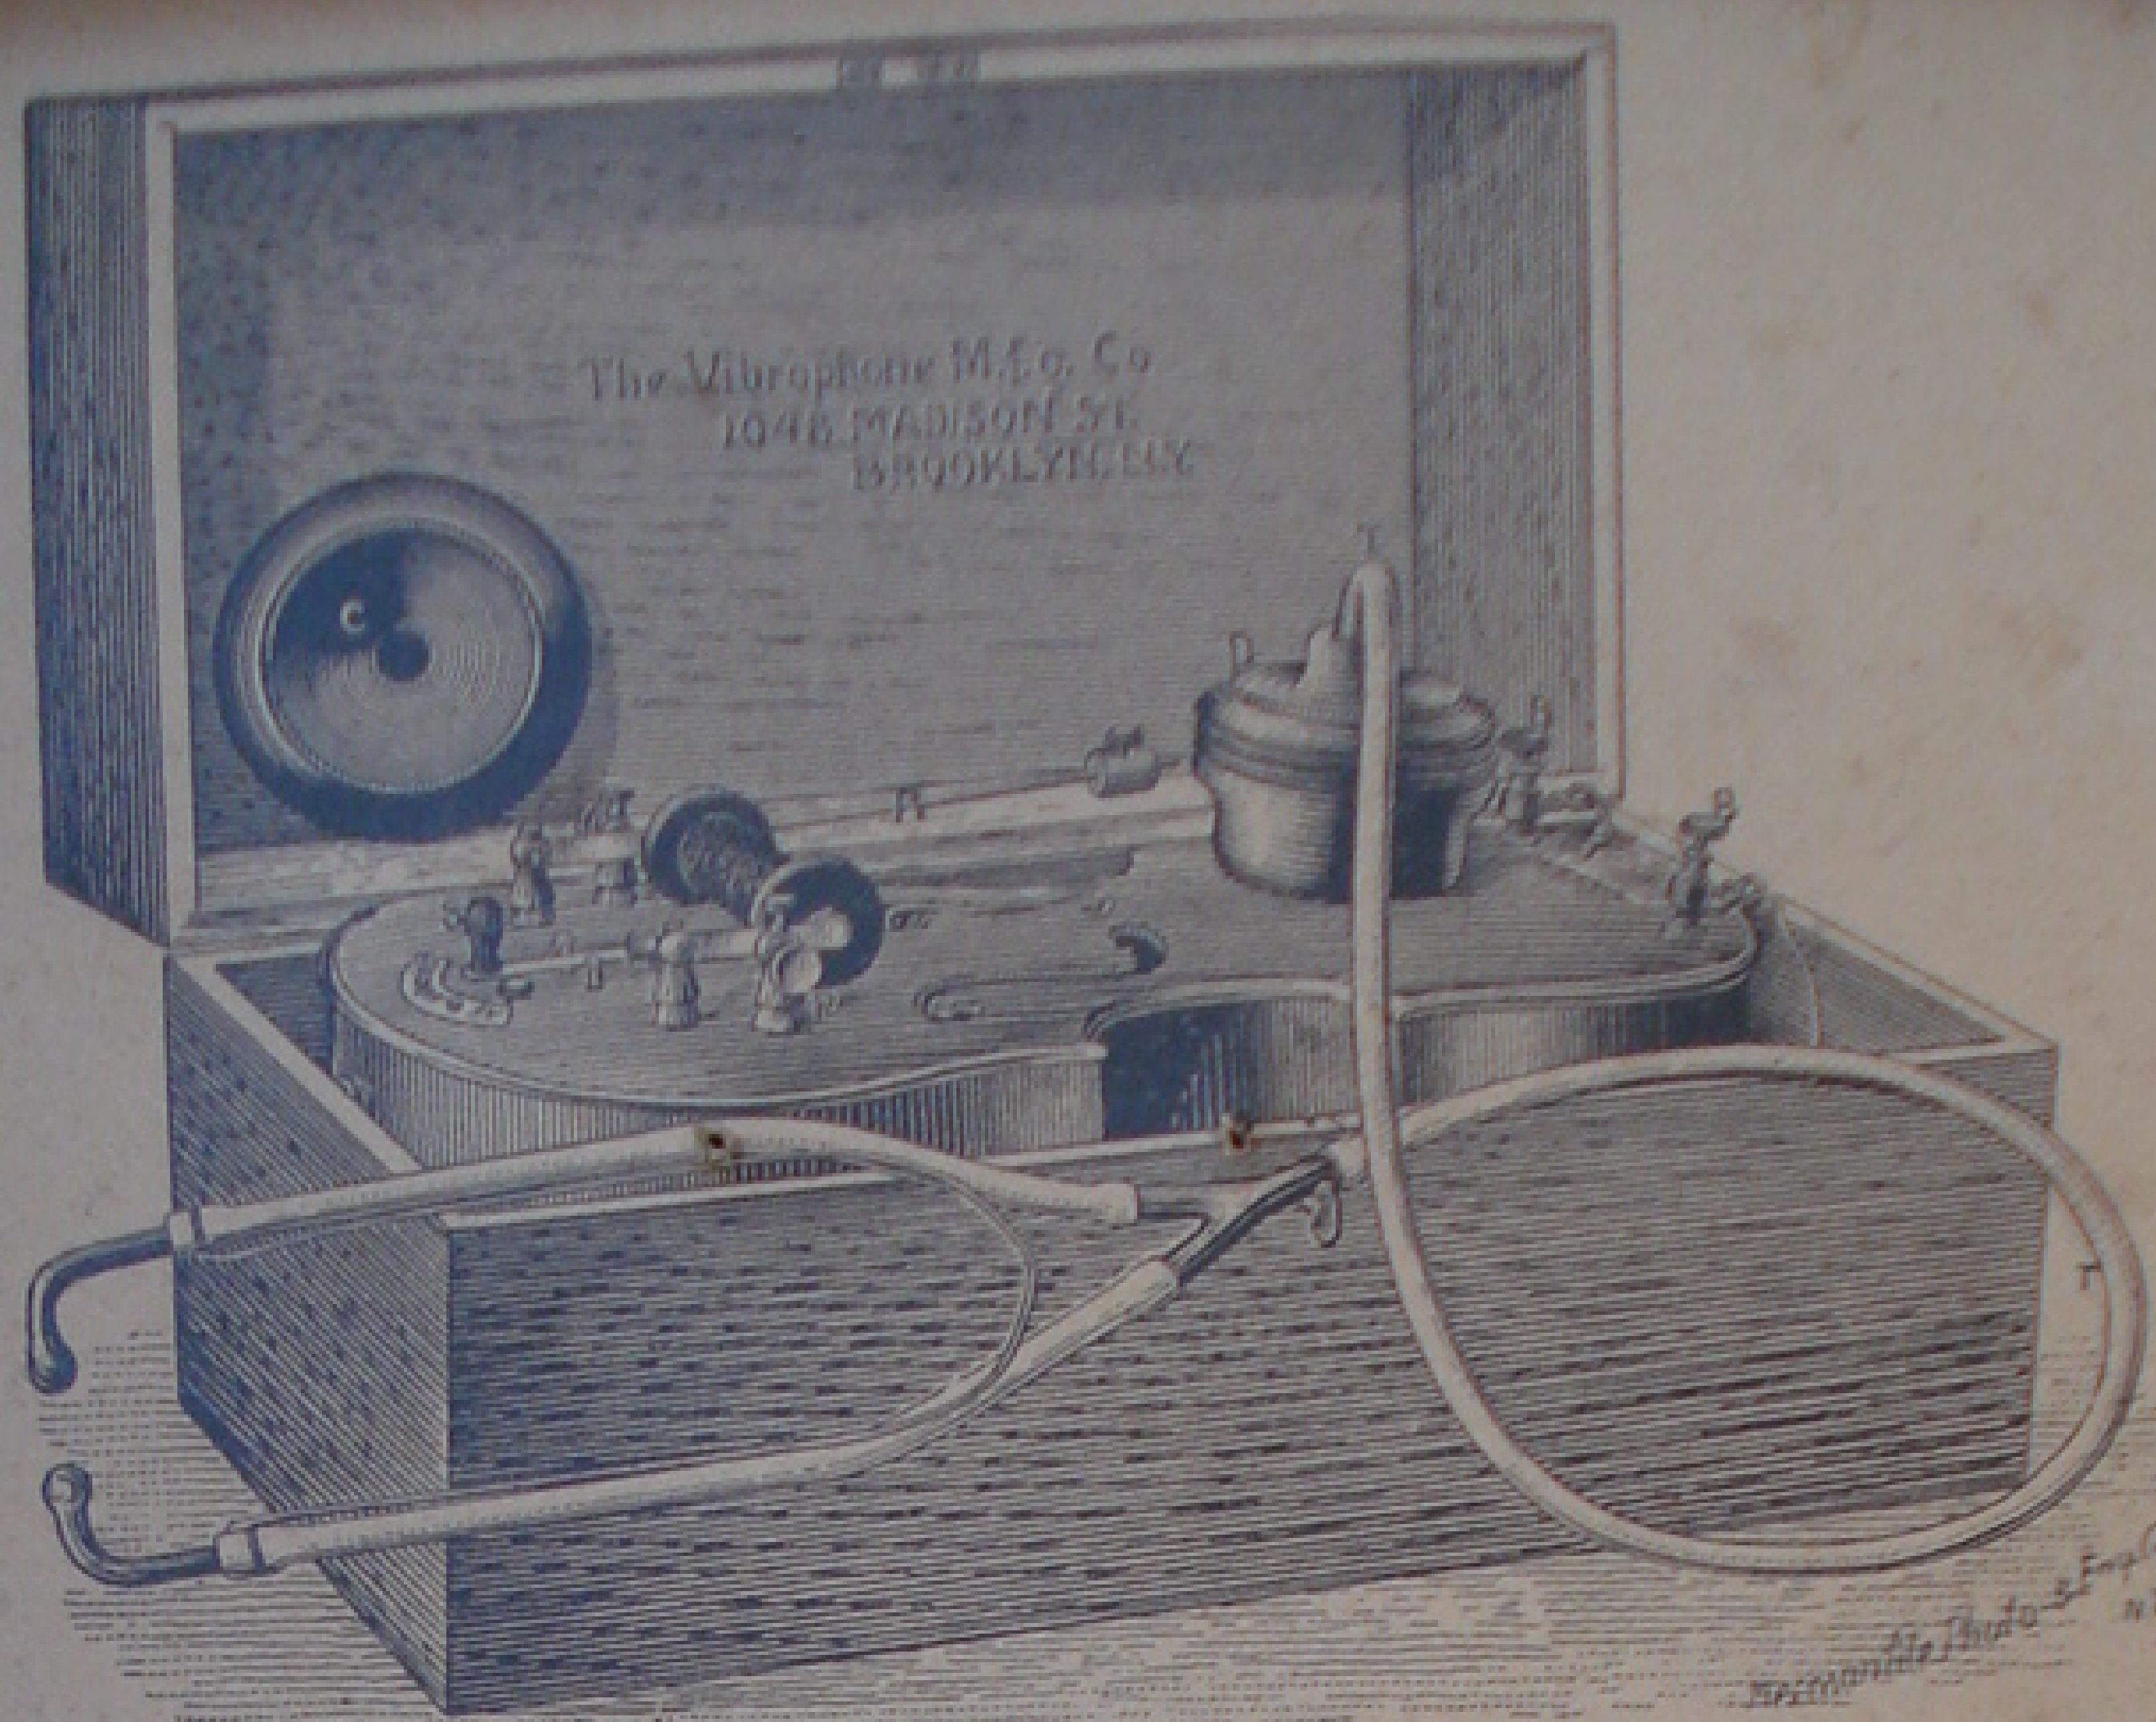

The Vibrophone Manufacturing Co.

1046 & 1048 MADISON STREET, BROOKLYN, N. Y.

DIRECTIONS FOR USING THE VIOLIN VIBROPHONE.

B, B, which is represented on cut, are the Binding posts to which the Batteries are connected by means of wire cable.

The Wire coil between the Binding posts is the Rheostate, with which the current is turned off, or on by turning switch on same, from right to left.

S is the swtich with which the vibrators are set in motion. For slow vibrations turn switch to S. V., for (low tuned) fast vibrations to M. V and for very fine vibrations (high C) to F. V. (see plate on Instrument.)

R, Rod, whereon slow vibrations are changed by changing position of ball, **P**, Platinum contact screws wherewith the sound of fast vibrators are changed, by either screwing same in or out. **D**, Receiver to which vibrations are conducted, wherein they are magnified and from which they are, by means of rubber Tubing **T**, conveyed to the Ears, **C**, Extra large upper part of Receiver used in Chronic Cases. To use same, remove small upper part of receiver and affix the large one in the same manner.

"**Caution!** Never short circut cells, by placing METAL against the two Binding posts, and never fail to have switch at OFF when Instrument is not in use.

The Platinum contacts on contact screw and vibrator should always be clean, to obtain regular vibrations.



The Vibrophone Manufacturing Co.

1046 & 1048 MADISON STREET,

BROOKLYN, N. Y.

DIRECTIONS FOR USING THE VIOLIN VIBROPHONE.

B. B. which is represented on cut, are the Binding posts to which the Batteries are connected by means of wire cable.

The Wire coil between the Binding posts is the Rheostate, with which the current is turned off, or on by turning switch on same, from right to left.

S is the swtich with which the vibrators are set in motion. For slow vibrations turn switch to S. V., for (low tuned) fast vibrations to M. V and for very fine vibrations (high C) to F. V. (see plate on Instrument.)

R, *Rod*, whereon slow vibrations are changed by changing position of ball, **P**, Platinum contact screws wherewith the sound of fast vibrators are changed, by either screwing same in or out. **D**, Receiver to which vibrations are conducted, wherein they are magnified and from which they are, by means of rubber Tubing **T**, conveyed to the Ears, **C**, Extra large upper part of Receiver used in Chronic Cases. To use same, remove small upper part of receiver and affix the large one in the same manner.

"**Caution!** Never short circut cells, by placing METAL against the two Binding posts, and never fail to have switch at OFF when Instrument is not in use.

The Platinum contacts on contact screw and vibrator should always be clean, to obtain regular vibrations.